DuraTracker[®] Installation and Operation Guide





69-4803-032 Revision: E, April 2024

© 2022 Teledyne Instruments Incorporated. All rights reserved.

Information included herein is controlled by the Export Administration Regulations (EAR) and requires an export license, license exception or other approval from the appropriate U.S. Government agency before being exported from the United States or provided to any foreign person. Diversion contrary to U.S. law is prohibited.

Foreword - Water and Wastewater Products

This instruction manual is designed to help you gain a thorough understanding of the operation of the equipment. Teledyne ISCO recommends that you read this manual completely before placing the equipment in service.

Although Teledyne ISCO designs reliability into all equipment, there is always the possibility of a malfunction. This manual may help in diagnosing and repairing the malfunction.

If a problem persists, call or e-mail Teledyne ISCO technical support for assistance. Simple difficulties can often be diagnosed over the phone. For faster service, please have your serial number ready.

If it is necessary to return the equipment to the factory for service, please follow the shipping instructions provided by technical support, including the use of the Return Merchandise Authorization (RMA) specified. Be sure to include a note describing the malfunction. This will aid in the prompt repair and return of the equipment. No item may be returned for service without a Return Merchandise Authorization (RMA) number issued by Teledyne.

Teledyne ISCO welcomes suggestions that would improve the information presented in this manual or enhance the operation of the equipment itself.

Teledyne ISCO is continually improving its products and reserves the right to change product specifications, replacement parts, schematics, and instructions without notice.

Contact Information

Custom	er Service				
	Phone:	(800) 228-4373	(USA,	Canada,	Mexico)
		(402) 464-0231	(Outside North And	merica)	
	Fax:	(402) 465-3022			
	Email:	isco.orders@teledyne.com			
Technical Support					
	Phone:	Toll Free (866) 298-	6174 (Samplers and	l flowmeters)	
	Email: iscowatersupport@Teledyne.com				
	Return equipment to:	4700 Superior Street	, Lincoln, NE 68504	4-1398	
Other C	orrespondence				
	Mail to:	P.O. Box 82531, Lin	coln, NE 68501-25	31	

Warranty and Operation Manuals can be found on our website at:

www.teledyneisco.com

EAR-Controlled Technology Subject to Restrictions Contained on the Cover Page

Before installing, operating, or maintaining this equipment, it is imperative that all hazards and preventive measures are fully understood. While specific hazards may vary according to location and application, heed the following general warnings:

Avoid hazardous practices! If you use this instrument in any way not specified in this manual, the protection provided by the instrument may be impaired.

Éviter les usages périlleux! Si vous utilisez cet instrument d'une manière autre que celles qui sont specifiées dans ce manuel, la protection fournie de l'instrument peut être affaiblie; cela augmentera votre risque de blessure.

This manual applies *Hazard Severity Levels* to the safety alerts. These three levels are described in the sample alerts below.

Cautions identify a potential hazard, which if not avoided, may result in minor or moderate injury. This category can also warn you of unsafe practices, or conditions that may cause property damage.

Warnings identify a potentially hazardous condition, which if not avoided, could result in death or serious injury.

DANGER – limited to the most extreme situations to identify an imminent hazard, which if not avoided, will result in death or serious injury.

Safety

Hazard Severity Levels

Hazard Symbols		nent and this manual use symbols used to warn he symbols are explained in the table below.		
		Hazard Symbols		
		Warnings and Cautions		
		The exclamation point within the triangle is a warning sign alerting you of important instructions in the instrument's technical reference manual.		
	<u>Á</u>	The lightning flash and arrowhead within the trian- gle is a warning sign alerting you of "dangerous voltage" inside the product.		
		Symboles de sécurité		
		Ce symbole signale l'existence d'instructions importantes relatives au produit dans ce manuel.		
	<u>Á</u>	Ce symbole signale la présence d'un danger d'électocution.		
	v	Warnungen und Vorsichtshinweise		
		Das Ausrufezeichen in Dreieck ist ein Warnze- ichen, das Sie darauf aufmerksam macht, daß wichtige Anleitungen zu diesem Handbuch gehören.		
	<u>Á</u>	Der gepfeilte Blitz im Dreieck ist ein Warnzeichen, das Sei vor "gefährlichen Spannungen" im Inneren des Produkts warnt.		
		Advertencias y Precauciones		
		Esta señal le advierte sobre la importancia de las instrucciones del manual que acompañan a este producto.		
	<u>Á</u>	Esta señal alerta sobre la presencia de alto vol- taje en el interior del producto.		

DuraTracker®

Table of Contents

Section 1 Introduction

1.1 Product Description
1.2 Compatible Equipment1-1
1.3 Input Voltage 1-2
1.4 Component Identification 1-4
1.5 Connector Receptacles 1-7
1.6 Maintenance 1-7
1.7 Unpacking Instructions 1-7
1.8 Technical specifications 1-8

Section 2 Preparation and Installation

2.1	Overview
	2.1.1 Safety
2.2	Modem Installation
	2.2.1 SIM Card
	2.2.2 Installing the LTE modem
	2.2.3 Magnetic-Mount Antenna 2-7
	2.2.4 Antenna Placement
	2.2.5 Modem Frequency Bands 2-8
	2.2.6 Modem Regulatory Compliance 2-9
2.3	Desiccant Inspection
	Communications
2.5	Permanent System Installation 2-11
	Portable System Installation
	Using a DuraTracker in Hazardous Location (with Barrier)
2.8	Mounting the DuraTracker
	2.8.1 Program the Module
2.9	Final Installation Check

Section 3 Programming

3.1	Overview
3.2	Flowlink Help 3-1
3.3	Flowlink Connections
	3.3.1 USB
	3.3.2 Bluetooth
	3.3.3 Modem
	3.3.4 Remote Updates
	3.3.5 Remote Data Retrieval
	3.3.6 SMS
	3.3.7 Datapush
	3.3.8 Check connection
3.4	Configuration
	3.4.1 Program Settings 3-10
	3.4.2 Site Name
	3.4.3 Devices
	3.4.4 TIENet Setup
	3.4.5 Data Storage Settings
	3.4.6 Applying Setting Changes 3-14

3.4.7 Time Resolution	3-14
3.4.8 Rollover Memory	3-14

Section 4 Modbus Output Protocol

4.1		4 1
4.1	Overview	1- 1
	Setup	
4.3	Operation	4-4
	4.3.1 Establishing Communication	4-4
	4.3.2 Module Addressing	4-4
	4.3.3 Configurations	4-4
4.4	Glossary of Terms	4-5
4.5	DuraTracker ASCII or RTU Address	4-7
4.6	Register Definitions	4-7
	4.6.1 Modbus Registers	4-7

Section 5 Maintenance

5.1 Overview
5.2 Maintenance Kits
5.3 Battery Maintenance
5.3.1 Battery Usage 5-1
5.3.2 Battery Usage Examples 5-2
5.4 Surcharging Precaution 5-6
5.5 Desiccant Maintenance 5-6
5.5.1 Replacing Desiccant 5-7
5.5.2 Reactivating Desiccant
5.6 Hydrophobic Filter Maintenance 5-8
5.7 Cleaning the DuraTracker 5-10
5.8 Servicing the DuraTracker 5-10
5.9 Diagnostics

Appendix A

A.1 Replacement Parts A	۱-1
A.2 Optional Equipment and Accessories A	\-1
A.2.1 Cables and Accesories A	\-1
A.2.2 Battery Options A	\-1
A.2.3 301 pH/Temperature Device Ending in TIENet Plug A	\-1
A.2.4 306 Sampler Interface Cable with Connection Ending in TIENet Plug A	\- 2
A.2.5 310 Ex Ultrasonic Level Sensor with Connection Ending in	
TIENet Plug	\- 2
A.2.6 360 LaserFlow Velocity Sensor with Connection Ending in TIENet Plug A	\- 2
A.2.7 360 LaserFlow Ex Velocity Sensor with Connection Ending in	
TIENet Plug	\- 3
A.2.8 350 Ex Area Velocity Sensor with Connection Ending in	
TIENet Plug	\- 3
A.2.9 Modems	
A.3 Company Contact Information A	\- 3
A.3.1 Customer Service Department A	

Appendix B Material Safety Data Sheets

B.1 SafetyB-

List of Figures

1-1 DuraTracker Front
1-2 DuraTracker Rear
1-3 DuraTracker w/o Battery Box 1-6
1-4 Capping the connector receptacle 1-7
1-5 Specification Drawing, DuraTracker with Battery Box 1-10
1-6 Specification Drawing, DuraTracker without Battery Box 1-11
2-1 Non-Hazloc Modem
2-2 Types of SIM cards
2-3 FCC ID label on modem and location of label on top of DuraTracker case 2-3
2-4 Screw removal
2-5 Disconnecting electrical connector and reference line 2-4
2-6 Screw removal
2-7 Plugging modem into circuit board 2-5
2-8 Connecting antenna cable 2-5
2-9 Installing SIM card
2-10 Screw tightening sequence
2-11 Magnetic Mount Antenna
2-12 Connecting a TIENet sensor cable
2-13 Power/Modbus Cable
2-14 Power/Modbus Connections 2-12
2-15 Installation of 6 volt lantern batteries 2-13
2-16 Installation of 1.5 VDC Alkaline D cell batteries 2-13
2-17 Installation of 3.6 VDC Lithium Thionyl Chloride D cell batteries 2-14
2-18 310 Ex Ultrasonic Sensor 2-14
2-19 350 Ex Area Velocity Sensor
2-20 360 LaserFlow Ex Sensor
2-21 360 LaserFlow Ex Sensor with Surcharge Sensor 2-15
3-1 USB installation
3-2 Flowlink connection screen 3-2
3-3 Flowlink Modem Tab 3-6
3-4 The UpdateSoftware Program
3-5 Data tab
3-6 Manual Data Push 3-9
3-7 301 pH and Temperature Sensor Parameters 3-12
3-8 306 Sampler Interface Parameters 3-12
3-9 310 Ex Ultrasonic Sensor Parameters 3-12
3-10 350 Ex Area Velocity Sensor Parameters 3-12
3-11 360 LaserFlow Sensor Parameters 3-12
3-12 360 LaserFlow Ex Sensor Parameters 3-13
3-13 Data Storage Setup window
4-1 Screw removal
4-2 Disconnecting electrical connector and reference line 4-2
4-3 Jumper position
4-4 Screw tightening sequence 4-3
4-5 Configuration example 4-5
5-1 Desiccant cartridge locations 5-6
5-2 Removal of Desiccant Cartridge Cap 5-7
5-3 Replacing the hydrophobic filter 5-8
5-4 Retrieving diagnostic files manually 5-10
5-5 Retrieving diagnostic files automatically 5-11

List of Tables

1-1	DuraTracker Battery Options		1-3
-----	-----------------------------	--	-----

1-2	DuraTracker Components - Front View	1-4
1 - 3	DuraTracker Components - Rear View	1-5
1-4	DuraTracker w/o Battery Box Components	1-6
1-5	DuraTracker Flow Meter Technical Specifications	1-8
2-1	Modem Frequency Bands	2-8
2-2	Power/Modbus Connections 2	-12
3-1	Site Window Tabs 3	-10
3-2	Invalid Characters 3	-10
4-1	Modbus Terms	4-6

DuraTracker®

Section 1 Introduction

1.1 Product Description

The DuraTracker flow logger and the attachable TIENet[™] devices are designed for open channel flow monitoring applications. It has built-in standard level-to-flow conversions that cover the majority of open channel flow measurement situations. Flow measurement is a calculation based on a known relationship between liquid level and flow rate. Additionally, the DuraTracker can calculate flow using standard open channel level-to-flow and area-velocity conversions, including equations and data points, depending on the measurement device(s) attached to the meter and the program specified by the user.

The DuraTracker's data storage memory can store measurement in intervals ranging from 15 seconds to 24 hours. It can also be configured for variable rate data storage to enable storage at differing intervals depending on the occurrence of programmed conditions. DuraTracker's program and collected data are stored on a flash memory microSD card for security. This retains data without the concern of power failures. The memory capacity of a microSD card is more than sufficient for most applications. For example, flash memory is capable of storing approximately 1.3 million readings — the equivalent of over 2700 days with 5 parameters at 15 minute intervals, reports once per day. Flash memory also stores instrument configuration and sensor calibration information.

The DuraTracker is programmed with Teledyne ISCO's Flowlink[®] software. Flowlink quickly configures the Dura-Tracker, retrieves measurement data, manages site information, and analyzes data.

DuraTracker's components are rated IP68. Its gasket-sealed enclosures are designed to meet the environmental demands of sewer flow monitoring applications. All connections between the DuraTracker's antenna and sensors lock in place. This locking mechanism secures the components and provides a watertight seal.

A basic DuraTracker system consists of two TIENet devices for flow and/or parameter measurement connected to the DuraTracker flowmeter. Other configurations may include an enclosure and additional internal or external devices. Dura-Tracker flowmeters can interface with a variety of measurement devices and other system components. Compatible flow measurement technologies include the TIENet 350 Continuous Wave Doppler Sensor, the TIENet 310 Ex Ultrasonic Level Sensor, and the TIENet 360 LaserFlow Sensor. Other compatible devices include the TIENet 301 pH & Temp Sensor, and the TIENet 306

1.2 Compatible Equipment

Sampler Interface. Four measurement devices for flow and water quality can be connected to the same DuraTracker and run simultaneously with TIENet connectivity. (See Section 3.4.3 for combinations that can be used.)

🗹 Note

For details on a TIENet sensor, refer to the user manual for that device.

For descriptions of interfacing and parameter-sensing TIENet devices, refer to Sections 2 and 3. Each external TIENet device comes with an individual user manual.

A variety of application-specific accessories are available from Teledyne ISCO. Refer to Appendix A.2 for a complete list of accessories and ordering information.

The DuraTracker power system's voltage measurement is used when estimating the remaining battery life and determining routine servicing. The voltage readings can be logged in data storage to chart power consumption.

The DuraTracker has two battery compartments that power the unit. Only one battery compartment is needed to run the unit. If both battery compartments are used, the DuraTracker will deplete the batteries in one compartment first before switching to the other battery compartment.¹

🗹 Note

360 LaserFlow battery banks will run in parallel at all times. It is recommended to use both banks of batteries when running a 360 LaserFlow.

The DuraTracker also has the option of using external power supplied through the Power/Modbus cable. When power is detected at the external source, the DuraTracker will always use that source.

1.3 Input Voltage

^{1.} See Section 5.3.1 *Battery Usage* for further information about battery bank-switching behavior.

Table 1-1	DuraTracker Batter	ry Options
6 VDC Alkaline Lantern Battery Rayovac 808	Requires two batteries in one bank to operate. An additional two bat- teries can be used to extend life.	Battery: 340406000 Holder: 604804025 (comes with two)
1.5 VDC Alkaline D Cell Battery	Requires eight batteries in one bank to operate. An additional eight bat- teries can be used to extend life. A HazLoc D cell battery holder can be ordered from Tele- dyne ISCO.	Holder: 604804024
3.6 VDC Spiral Wound Lithium Thionyl Chloride D Cell Battery (non- Rechargeable)	Requires four batteries. An additional four can be used to extend life. A custom Lithium D cell battery holder can be ordered from Teledyne ISCO.	Battery: 340903600 Holder: 604804026

1.4 Component Identification

The components of the DuraTracker are shown in Figure 1-1, Figure 1-2 and Figure 1-3. Items referenced in those figures are summarized in Table 1-2, Table 1-3, and Table 1-4.



Figure 1-1 DuraTracker Front

Ta	Table 1-2 DuraTracker Components - Front View				
Item No.	Name	Description			
1	Antenna Connector	Used to connect the modem to the antenna			
2	USB Connector	The USB connector is used to connect the DuraTracker to a computer using a USB cable			
3	TIENet Connector	Used to connect the DuraTracker to compatible TIENet equipment			
4	Power/Modbus Connector	Used to connect the DuraTracker to external power and Modbus			
5	Hanging Bracket	Used to hang the DuraTracker			

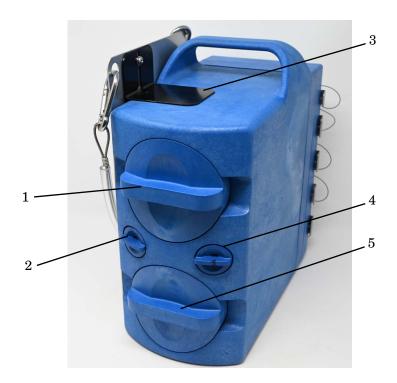


Figure 1-2 DuraTracker Rear

Ta	Table 1-3 DuraTracker Components - Rear View				
Item No.	Name	Description			
1	Battery Cap Bank 1	Used to secure the battery in the DuraTracker			
2	Desiccant Cap (reference air and electronics)	Used to secure the desiccant for the reference air and electronics hous- ing in the DuraTracker			
3	Antenna Mount Bracket (optional)	Used to locate the antenna on the DuraTracker			
4	Desiccant Cap (battery box)	Used to secure the desiccant for the battery box in the DuraTracker			
5	Battery Cap Bank 2	Used to secure the battery in the DuraTracker			



Figure 1-3 DuraTracker w/o Battery Box

Tabl	Table 1-4 DuraTracker w/o Battery Box Components					
Item No.	Name	Description				
1	Antenna Connector	Used to connect the modem to the antenna				
2	USB Connector	The USB connector is used to connect the DuraTracker to a computer using a USB cable				
3	TIENet Connector	Used to connect the DuraTracker to compatible TIENet equipment				
4	Power/Modbus Connector	Used to connect the DuraTracker to external power and Modbus				
5	Antenna Mount Bracket (optional)	Used to locate the antenna on the DuraTracker				
6	Hanging Bracket	Used to hang the DuraTracker				
7	Desiccant Canister	Used to hold desiccant for the reference air and electronics housing in the DuraTracker				

1.5 Connector Receptacles

Any connector receptacle not in use should always be capped. The cap seals the connector in order to prevent moisture from entering the unit and corrosion from occurring.

☑ Note

Caps push on and pull off. Do not rotate the caps to remove them from the connectors. Always push caps into the receptacle until you hear an audible click. The click occurs when the latch locks the cap in place.



Figure 1-4 Capping the connector receptacle

1.6 Maintenance

The DuraTracker is designed to provide durable operation with minimal routine maintenance. All maintenance can be performed in the field. Typically, maintenance consists solely of the replacement of desiccant and batteries. See Section 5 for more details.

1.7 Unpacking
InstructionsWhen the system arrives, inspect the outside packaging for any
damage. Then, carefully inspect the contents of the package for
damage.

If there is any evidence that items may have been damaged in shipping, do not attempt to install the unit. Contact Teledyne ISCO immediately.

When unpacking the system, check the contents with the included packing list. If any parts are missing, contact Teledyne ISCO's Customer Service Department. Contact information for Teledyne ISCO's Customer Service Department can be found in Appendix A.3.1. Please report missing part(s) by part number. In addition to the primary packing list, there may be secondary packing lists for various sub-components. It is recommended that you retain the shipping cartons, as they can be used to return the unit to Teledyne ISCO if necessary.

Please complete the registration card for the unit and return it to Teledyne ISCO.

1.8 Technical specifications

Table 1-5 D	uraTracker Flo	w Meter Tech	nnical Spec	ifications	
Size (HxWxD) DuraTracker DuraTracker w/o Battery Box	12.25 x 6.25 x 12. 13.375 x 8.625 x 4				
Weight DuraTracker DuraTracker w/o Battery box	14.3 lbs. (6.49 kg) 5.3 lbs. (2.4 kg)) without batterie	s		
Enclosure	IP68 (self certified	l for 6 feet (2 me	ters) for 24 ho	ours) ^a	
Power DuraTracker	9-15 VDC				
External Power (DuraTracker Ex does not have external power)	7-28 VDC				
Operating Temperature DuraTracker	-40° to 140 °F (-40° to 60 °C)				
Storage Temperature	-40 to 140 °F (-40	to 60 °C)			
Typical Battery Life			310 Ex Ultrasonic sensor	350 Ex AV Sensor	360 Ex LaserFlow sensor
	DuraTracker with*	2 x 6V Rayovac 808 Batteries	18 months	8 months	9.4 months
		D Cell Batteries	13.5 months	6 months	7 months
Data Storage	Non-volatile flash; retains stored data during program updates. Capacity 8 MB (1.3 million readings or 2700 days with 5 parameters logged at 15 minute intervals, reports once per day)				
Storage mode	Rollover, 5 bytes per reading				
Storage Interval	15 or 30 seconds; 1, 2, 5, 15 or 30 minutes; or 1, 2, 4, 12 or 24 hours. Storage rate variable based on measurement parameters				
Data Types	Flow Rate, Level, Temperature, Velocity, Volume, Input Voltage, Wireless Sig- nal				

Flow Measurement Technologies	Ultrasonic (TIENet 310 Ex) Continious Wave Doppler Velocity (TIENet 350) Laser Doppler Velocity TIENet 360 LaserFlow)
Flow Conversions	Weir, Flume, British Flume, Metering Insert, Manning Formula, Equation, LTF or LTA Data Points (up to 50 pairs), Area Velocity
Industry Standard Outputs	RS485 Modbus ASCII and RTU
Communication Options	Direct USB Serial Connection, 4G LTE Modem, Bluetooth

a. IP68 rating does NOT imply resistance to intrusion in cases of frequent surcharge events, prolonged submersion (greater than 24 hours) at lower than rated depths, or short duration submersion at depths greater than 2 meters.

*Actual battery life will vary depending on configuration. The figure given assumes interrogation on site with Flowlink once a week, with a site configuration as indicated and using one bank of batteries (two banks of batteries will double the battery life). The DuraTracker was configured to record level, velocity and flow rate every 15 minutes; total flow and battery voltage every 24 hours. No modem or Bluetooth connectivity.

🗹 Note

Never mix old and new batteries. Never mix different types of batteries. Never mix batteries from different manufacturers.

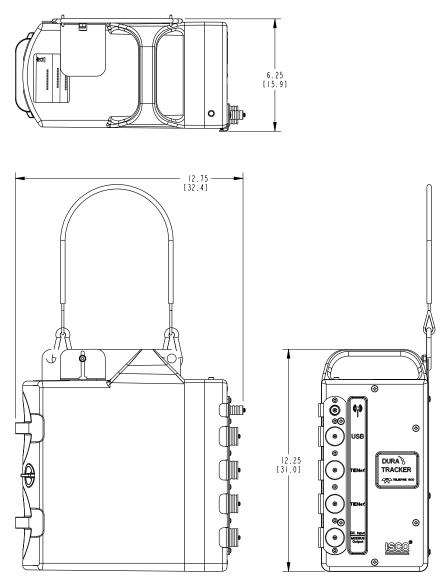


Figure 1-5 Specification Drawing, DuraTracker with Battery Box

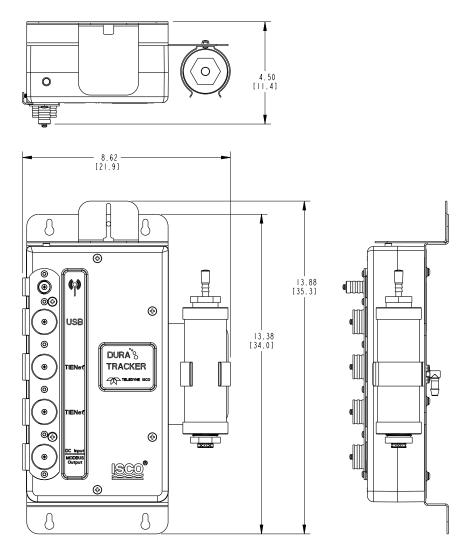


Figure 1-6 Specification Drawing, DuraTracker without Battery Box

DuraTracker®

Section 2 Preparation and Installation

2.1 Overview	The section covers preparation instructions for the installation of the DuraTracker and is not for the DuraTracker Ex.
	The DuraTracker flow meter may be installed as a permanent or as a portable system. Permanent systems are powered by the power input cable as described in Section 2.5. Portable systems are powered by battery power as described in Section 2.6.
	Avoid hazardous practices! If you use these instruments in any way not specified in this manual, the protection provided by the instruments may be impaired. This will increase your risk of injury.
2.1.1 Safety	Before installing, operating, or maintaining the equipment, it is imperative that all hazards and preventative measures are fully understood.
Site Conditions	The DuraTracker components are often installed in confined spaces. Examples of confined spaces include manholes, pipelines, digesters, and storage tanks. These spaces may become haz- ardous environments that can prove fatal for those unprepared. In the United States, these spaces are governed by OSHA 1910.146 and require a permit before entering. For areas outside of the United States, adhere to local laws and safety regulations concerning confined space entry.
	The installation and use of this product may subject you to hazardous working conditions that can cause you serious harm or fatal injuries. Take any necessary precautions before entering a worksite. Install and operate this product in accordance with all applicable safety and health regulations, and local ordinances.
Mounting Considerations	Ideal installation sites for the DuraTracker are easily accessible for service and data collection while still providing protection for the device. The DuraTracker is constructed of materials that can withstand hard environments. However, continual exposure to UV light or periodic submersion should be avoided in order to extend the life of the components.
	Typically, the DuraTracker is suspended inside a manhole. Suspending it near the opening will protect it from the elements, minimize the chance of submersion, and allow it to be easily retrieved without entering the manhole.

System Power

The maximum voltage for the DuraTracker is 15 V in the battery compartment and 28 V from the external power plug.

Injury and/or equipment damage can result from attempting to connect a DuraTracker to a system using a power source that exceeds the specified operating voltage range. Check labeling on all units and cables for voltage ranges.

2.2 Modem Installation The Long Term Evolution (LTE) modems can automatically push data to a secure server running ISCO Flowlink Pro software. With LTE data transmission, your service parameters or provider can be changed by replacing the removable Subscriber Information Module (SIM) card in your modem. There is one modem for North America and one for Europe.



Figure 2-1 Non-Hazloc Modem

2.2.1 SIM Card

The data transmission capabilities of the LTE modems are dependent upon the type of service plan you have through your cell phone service provider. The service parameters, or provider, can be changed by simply replacing the SIM card in your modem. Check with your service provider to verify which data transmission technologies are available for your use. There are three types of SIM cards, but only Micro SIM cards will work in the LTE modems.

🗹 Note

A Micro SIM card is required for any LTE units including the DuraTracker modems.



Figure 2-2 Types of SIM cards


🗹 Note

If you are using Verizon and want to be able to text the modem, you MUST use Verizon SIM card P/N BULKSIM-TRI-A or Nimbelink SIM card P/N NL-SIM-COM due to Verizon LTE network not having fallback to 2G/3G.


2.2.2 Installing the LTE The modem kit includes the modem, antenna, and antenna bracket with hardware.

Mote

Before installing the modem, remove the top label (with the FCC ID and IMEI number on it) taped to the modem and adhere it to the outside of the DuraTracker case on the top of the unit, next to the antenna bracket (See Figure 2-3). This is required by the FCC and ensures the IMEI number is visible.

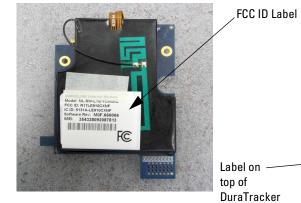





<u> ✓ Note</u>

The DuraTracker modem will not work in the DuraTracker Ex.

case

1. Remove batteries from DuraTracker and open the front electronics panel by removing the six screws on the front of the unit. Before opening the case, make sure you are grounded so that you do not damage the internal components with an Electrostatic Discharge (ESD).



Figure 2-4 Screw removal

If case is opened to install a modem, change a SIM card, or set up Modbus, ESD protection must be observed. Failing to do so could result in damage to the DuraTracker.

🗹 Note

Do not install screws using power tools. Use only hand tools

2. Open the case and disconnect the electrical connector and reference line from the battery box.



Figure 2-5 Disconnecting electrical connector and reference line

3. Remove the two screws from the upper left section of the DuraTracker case and set them aside to reuse.



Figure 2-6 Screw removal

4. Connect the new modem to the circuit board by lining up the connectors and pushing the board all the way down.



Figure 2-7 Plugging modem into circuit board

- 5. Reinstall the two screws that were removed in step 3 through the modem to hold it in place.
- 6. Connect the antenna connector to the modem and tighten all the way down.



Figure 2-8 Connecting antenna cable

7. Install the SIM card in the SIM card holder with the notch facing out.



Figure 2-9 Installing SIM card

- 8. Line up the two halves of the case, being careful to make sure the wires from the electrical connector do not get pinched between the two halves.
- 9. Reattach the front panel with the screws removed in step 1.
 - a. Insert all of the previously removed screws into the holes. "Start" the screws to line up the threads of the screws to the threads of the hole. Do not fully tighten them until Step b.
 - When starting screws in plastic, you should always first turn them counterclockwise until you feel/hear the audible click of the threads lining up. Once the threads line up, you can then turn the screw clockwise to tighten it down. This will ensure that you do not cross thread the plastic holes.
 - b. Tighten the screws in the sequence shown in Figure 2-10. This will ensure that the gaskets are tightened properly to maintain a watertight seal.
 - Repeat the sequence twice: first, tighten the screws enough to firmly hold the front half in place on the enclosure. Then, repeat the sequence to make the screws snug.

Don't cross thread the screws. Always follow the tightening procedure above. Failure to tighten the screws correctly could result in water infiltration and damage to the DuraTracker.




Figure 2-10 Screw tightening sequence

10. Install antenna bracket to the hanging bracket using the included hardware.

2.2.3 Magnetic-Mount Antenna The magnetic -mount antenna, included with LTE modems, has a 10-foot cable and a white connector indicating that it is suitable for LTE use. This antenna is for general use and is especially desirable when the system is housed within an enclosure.



Figure 2-11 Magnetic Mount Antenna

🗹 Note


When any communications connector is not in use, it should always be capped. The cap will seal the connector to prevent corrosion, prevent moisture from entering the unit, and improve communications.

2.2.4 Antenna Placement

1. The antenna needs to be placed in vertical orientation. It does **NOT** radiate out of the ends of the antenna.



- 2. The best performance will be with the antenna placed on a large metal ground plane, above ground and without large obstructions between the antenna and the tower. This is not always possible but in instances where signal strength is low, this may be necessary.
- 3. Any metal surrounding the antenna will degrade performance! Placing the antenna 4" to 8" lower than the metal ring the manhole cover sits on will provide better signal quality. Dirt and concrete lower signal strength less than metals which cause the signal to attenuate.

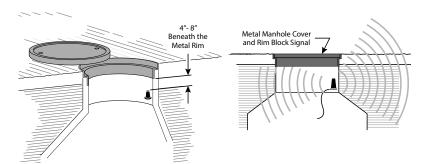

- 4. **Do NOT kink the coax!** The coaxial cable that feeds the antenna should never be in a loop tighter than the size of a fist. A coax that has been kinked will degrade the signal even after being straightened back out.
- 5. Antennas near strong radio towers or other sources of RF interference can jam the signal even though it is on a different frequency.

2.2.5 Modem Frequency Bands

	Table 2-1 Modem Frequency Bands				
ISCO Part Number	Туре	4G LTE Bands	Fallback	Applicable Networks	Location

Table 2-1 Modem Frequency Bands						
604807013	Cat 4	LTE-FDD: B2, B4, B5, B12, B13, B14, B66, B71	3G HSPA+: B2, B4, B5	AT&T, Verizon, Bell Telus and Rogers	North America and others, depending on supported bands	
604807014	Cat 4	LTE-FDD: B1, B3, B7, B8, B20	3G: B1, B8 2G: GSM 900, DCS 1800	Orange, Telstra, Telus, Vodafone and More	Europe and others, depending on supported bands	

2.2.6 Modem Regulatory Compliance

United States

Device Uses Approved Radio: NL-SW-LTE-TC4NAG Contains FCC ID: R17LE910CXNF Contains IC: 5131A-LE910CXNF

This device complies with Part 15 of the FCC Rules and Industry Canada license-exempt RSS standards. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Europe

This device has been Radio Equipment Directive tested and complies with EN 55011:2016/A1:2017/A11:2020 and EN 61326-1:2013.

CE

2.3 Desiccant Inspection Two desiccant cartridges are inserted into the battery compartment of the DuraTracker. The cartridges are filled with silica gel beads that will indicate when they are saturated. Under dry conditions, the beads are orange in color. As the desiccant becomes saturated, the beads turn green. If the entire length of the desiccant cartridge turns green, the unit is no longer adequately protected. Replace the desiccant before the entire length of the desiccant cartridge turns green. Refer to Section 5.4 for instructions on how to replace the desiccant cartridge.

> Inspect the color of the desiccant before deploying the unit or whenever on site. If monitoring the site remotely, periodically inspect the reference line humidity levels. If this level reaches an abnormally high humidity, visit the site to inspect the desiccant.

2.4 Communications The DuraTracker is accessed for configuration and data retrieval using Flowlink software. Connections between a PC and the DuraTracker can be made using a USB cable, Bluetooth[®], or via an IP address with a cellular modem. With Flowlink, you can name the site, set up its operation, adjust the level measurement

technologies, and retrieve stored measurements. To assist with servicing, Flowlink will display input power voltage (indicating remaining battery life) and collect diagnostic reports.

🗹 Note

To ensure protection of the unit, unused communication ports must be capped.

The DuraTracker has two TIENet receptacles located on the front of the unit. Sensor cables are attached to these receptacles. To connect the sensor:

- 1. Remove the protective caps.
 - a. Push down on the sensor release while pulling the protective cap from the TIENet receptacle.
 - b. Pull the cap from the end of the sensor cable plug.
- 2. Prepare the TIENet plug.
 - a. Inspect the plug. It should be clean and dry. Damaged O-rings must be replaced. Spare O-rings are supplied in the maintenance kit.
 - b. Coat the O-ring's sealing surface with a silicone lubricant.

Do not use petroleum-based lubricants. Petroleum-based lubricants will cause the O-ring to swell and prematurely deteriorate. Aerosol silicone lubricant sprays often use petroleum-based propellants. If using an aerosol spray, allow the propellant to evaporate for several minutes before proceeding.

Only plug sensors into the DuraTracker when power has been removed. Failure to do so could result in damage to the DuraTracker.

- 3. Insert the TIENet plug into the receptacle. The sensor release will click when the sensor cable is properly connected.
- 4. Connect the two caps.

TIENet Connections

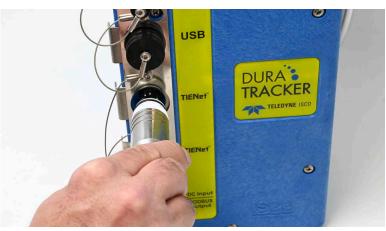


Figure 2-12 Connecting a TIENet sensor cable

Modbus Output Device

2.5 Permanent System Installation

The Modbus RS-485 output function enables a SCADA system to retrieve site data from the logger. The connection to a Modbus output device is achieved through the Power/Modbus Cable (ISCO P/N 604804023) shown in Figure 2-13 below. Connection information can be found in Figure 2-14 and Table 2-2.

For Modbus register numbers and definitions, as well as a general explanation of Modbus output protocol, refer to Section 4.

The DuraTracker front panel has a DC Input/Modbus Output connector port that can provide power to the unit. When power is provided via the DC Input, it will take precedence over the batteries as long as the DC Input power is higher than the batteries. Otherwise it will run on battery power until the battery bank in use is lower than the DC Input power. If batteries are installed, they will only be used in case the external power is removed or goes out. A Power/Modbus cable (ISCO Part# 604804023) is available from Teledyne ISCO customer service. The Power/Modbus cable plugs into the front panel of the Dura-Tracker and provides a watertight seal. The Power/Modbus cable can be used to supply up to 28 VDC to the DuraTracker.



Figure 2-13 Power / Modbus Cable

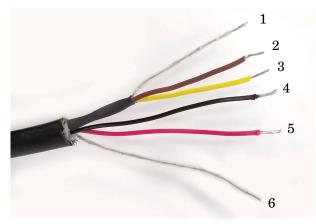


Figure 2-14 Power / Modbus Connections

	Table 2-2 Power/Modbus Connections				
Item No.	Name	Description			
1	Shield	Tied to Ground			
2	Brown	D0 (-)			
3	Yellow	D1 (+)			
4	Black	Ground			
5	Red	Positive			
6	Braid-Drain	Earth Ground			

2.6 Portable System Installation

The DuraTracker battery compartment has two banks for batteries. Each bank can provide power to the unit independently of the other bank. The DuraTracker can use a variety of battery options as detailed in Table 1-1. The figures below show the installation procedure for each of these battery options.







Figure 2-15 Installation of 6 volt lantern batteries



Figure 2-16 Installation of 1.5 VDC Alkaline D cell batteries

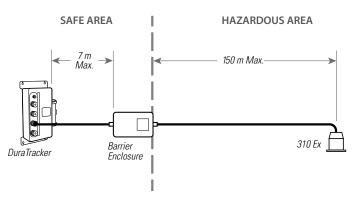



Figure 2-17 Installation of 3.6 VDC Lithium Thionyl Chloride D cell batteries.



2.7 Using a DuraTracker in Hazardous Location (with Barrier)

The DuraTracker may be used in a Hazardous location if a Teledyne ISCO Barrier (ISCO P/N 604364112) is used to connect to the sensor. The Barrier must be set up following its control drawing (see the TIENet Barrier manual for details). When using a 350 Ex, a Ex Reference Air Box must be used (see the 350 Ex manual for details). See the following diagrams for maximum cable lengths and configurations for Hazardous locations when using a DuraTracker and Barrier.





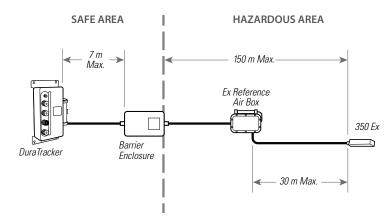


Figure 2-19350 Ex Area Velocity Sensor

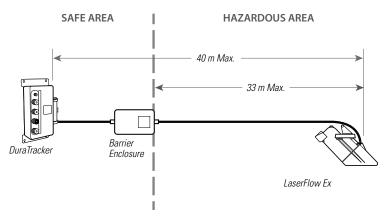


Figure 2-20360 LaserFlow Ex Sensor

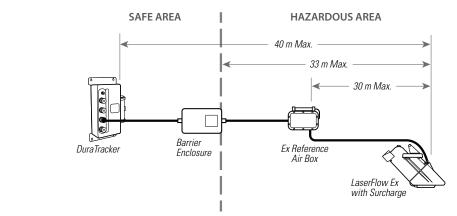


Figure 2-21360 LaserFlow Ex Sensor with Surcharge Sensor

2.8 Mounting the DuraTracker	
Site Examples	The DuraTracker is designed to monitor flow in open channels. The unit should be secured at the site. This prevents damage caused by accidental falls and from being swept away if the channel is flooded. A typical installation involves having the logger suspended from a manhole ladder or other support. Other options include the use of a spreader bar. Teledyne ISCO's Product Support Services Group or your local representative can assist you with installation options.
	Additionally, there will need to be a selection made as to the appropriate mounting hardware for the TIENet sensor.
2.8.1 Program the Module	After you have installed the Sensor, the flow stream properties must be defined. To do this, connect to the DuraTracker with Flowlink for Windows software and define the stream properties in the DuraTracker's program settings. These ensure that the system correctly reads the liquid level and converts the mea- sured level to flow rate.
	Note
	The DuraTracker requires Flowlink 5.19 or later. Earlier versions do not support the DuraTracker.
2.9 Final Installation Check	Basic Installation Checklist - As a review, the following steps may be used as a guide to install a DuraTracker at a basic site.
	1. Install the TIENet Sensor per the sensor manual.
	2. Attach the TIENet Sensor cable to the DuraTracker.
	3. Prepare the Battery Box.a. Install batteries.b. Inspect desiccant.
	4. Connect to the site with Flowlink Softwarea. Create the site by Quick Connecting to the modules.b. Set up the site and DuraTracker settings.c. Calibrate the level measurement.
	5. Disconnect from the site and replace all protective caps.
	6. Mount or suspend the DuraTracker.
	Only plug sensors into the DuraTracker when power has been removed. Failure to do so could result in damage to the Dura-Tracker.

DuraTracker®

Section 3 Programming

3.1 Overview	This section describes how to set up the operation parameters for the DuraTracker using Teledyne ISCO's Flowlink software.
3.2 Flowlink Help	This user manual contains basic Flowlink help and procedures. Detailed Flowlink instructions are available in Windows Help format. You can access the help topics for an active window within Flowlink by clicking on the Help button or by pressing F1 on your computer's keyboard. You can also access Help from the Flowlink menu by selecting HELP > CONTENTS AND INDEX. These instructions are provided within the Flowlink software user manual.
3.3 Flowlink Connections	Initial connection to the DuraTracker is made directly between a PC and the unit using a USB connection cable or Bluetooth connection and Teledyne ISCO's Flowlink software. After the initial connection and setup of the modem, subsequent connections can also be made via a modem connection (IP).
3.3.1 USB	Push the lock release on the port labeled USB and pull the cap off the front panel without twisting the cap. Plug the USB B male con- nector into the port on the DuraTracker and the USB A male to a PC of the connection cable. The DuraTracker is now ready to be logged into via Flowlink software.



Figure 3-1 USB installation

3.3.2 Bluetooth


Enabling Bluetooth


In order to connect to a DuraTracker unit via Bluetooth, the Bluetooth module on the unit must first be powered. To do this, the user may connect to the DuraTracker unit with Flowlink and define a Bluetooth control schedule from the Wireless Power Control tab. (Setting the Bluetooth control schedule will affect battery life.) Alternatively, power cycling the DuraTracker unit by removing all batteries for 60 seconds and then reinstalling them will enable Bluetooth for a 20 minute duration after power is applied to the unit.

If the DuraTracker has a modem and it has been set up already, you can text the word "Bluetooth" to the phone number and the DuraTracker will text back and open a 20 minute window once the text has been read by the unit. The SMS checking interval is set in Flowlink, but the default is 1 hour (at the top of every hour.) Setting the SMS check interval to less than 1 hour will affect battery life.

Once the DuraTracker Bluetooth module is powered, you can connect your device with the DuraTracker. Anytime the Bluetooth is actively powered, the LED on top of the unit will flash blue around once every 3 seconds.

Open Flowlink and access the Connect window. Select BLUE-TOOTH for connection type and click on the DISCOVER button. Once the DuraTracker is discovered it will show up in the drop-down list. Select your DuraTracker and click on the Dura-Tracker connection button. Flowlink will proceed to connect to your DuraTracker.

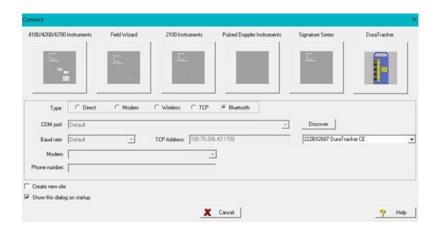



Establishing a Bluetooth

connection from Flowlink

Establishing a Bluetooth connection from a terminal emulator With a terminal emulator program, select the COM port corresponding to the DuraTracker unit, and use the following serial line settings:

- Speed: [doesn't matter]
- Data bits: 8
- Stop bits: 1
- Parity: none
- Flow control: none

Regulatory Approval

United States

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy, and if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Contains transmitter module FCC ID: A8TBM78ABCDEFGH in compliance with FCC rules.

FC

Canada

This device contains license-exempt transmitter(s)/ receiver(s) that comply with Innovation, Science and Economic Development Canada's license-exempt RSS(s). Operation is subject to the following two conditions:

- 1. This device may not cause interference;
- 2. This device must accept any interference, including interference that may cause undesired operation of the device.

L'émetteur/récepteur exempt de licence contenu dans le présent appareil est conforme aux CNR d'Innovation, Sciences et Développement économique Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes:

- 1. L'appareil ne doit pas produire de brouillage;
- 2. L'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

Contains transmitter module IC: 12246A-BM78SPPS5M2 that comply with Innovation, Science and Economic Development Canada's license-exempt RSS(s).

Europe


This device has been Radio Equipment Directive tested and complies with EN 55011:2016/A1:2017/A11:2020 and EN 61326-1:2013.



Japan



Korea



Taiwan



注意 ! 依據 低功率電波輻射性電機管理辦法 第十二條 經型式認證合格之低功率射頻電機, 非經許 可, 公司、商號或使用者均不得擅自變更頻率、加大功率或 變更原設計 之特性及功能。 第十四條 低功率射頻電機之使用不得影響飛航安全及 干擾合法通信; 經發現有干擾現象時,應立即停用,並改善至無干擾時 方得繼續使用。 前項合法通信,指依電信規定作業之無線電信。 低功率射頻電機須忍受合法通信或工業、科學及醫療用 電波輻射性 電機設備之干擾。

China

This device contains SRRC approved Radio module CMIIT ID: 2015DJ7133

United Kingdom

UK CA

3.3.3 Modem

Once the modem has had an Access Point Name (APN) entered into the appropriate field, the DuraTracker is able to be connected to by the modem if it has a static IP address. The Dura-Tracker can be set up with a call-in window to be able to access the unit at specific times, but this decreases battery life since it is on at the same times whether the unit is being contacted or not. The DuraTracker automatically turns on a 20 minute call window each time the power is cycled (by removing all batteries for 60 seconds). The user can also send the SMS message "status" to the units phone number and it will turn on a 20 minute call window once it reads the SMS message. The DuraTracker has a setting for how often it wakes up to check for SMS messages that can be set to 15 minutes, 30 minutes, 1 hour, 2 hours, 4 hours, 12 hours, or 24 hours.

Mote

Default is set to 1 hour, which results in the DuraTracker checking SMS messages at the top of every hour.

nfo De	evices Mea	T Goodyear asurements D		evel Alarms		neasurement tab >> Control ADFM Mo		32 AM - Connected Output Modem TIENet
	ound Contact Conr	ection Mode:	IP	▼ Port	1700	Service Provid	er Verizon	-
	APN:	mw01.VZW		_	1	150.230.247		
ι	Username:			Phor	ne number: +14	023109270		
F	Password:			Sign	al strength: 83	%		
E	Start Date: End Date: Send to N	6 / 7 /2021 6 / 7 /2021 Notification Grou	-	12:00:00 AM : 11:59:59 PM :	S	tart Manual Data Pus	h	
SM	S ext Retrieval	Interval: 15	i minutes 🔄]				

Figure 3-3 Flowlink Modem Tab

3.3.4 Remote Updates

Using a computer with Flowlink installed and an appropriate cellular service, you can access your remote monitoring site to remotely update the firmware. Bundled along with Flowlink is the UpdateSoftware program that can be used to achieve this. The DuraTracker must already have a call window set up, or you can send the SMS message "status" to the units phone number; then it will turn on a 20 minute call window once it reads the SMS message. Default SMS setting in Flowlink is 1 hour, so the SMS message would be checked at the top of the next hour. The return SMS message will contain the DuraTracker plus the last 3 digits of the serial number, site name, IP Address, and Status. After opening the UpdateSoftware program, enter the IP Address in the Modem section and click Connect. Once you have logged into the DuraTracker, just follow the prompts to update the firmware with the new firmware file that you previously downloaded from the Teledyne ISCO website.

Dpdate Software—v1.01.001 (351	a5bbe)		-	□ ×
Update	Softwar	е	0	2000
Connect	Select Device	Select File		
			\frown	
		\sim		~
Rodem				
IP Address	Por	t		
127.0.0.1	1	700		
			Connect	
				ப் Exit
TELEDYNE ISCO Everywhereyoulook*				1.01.001

Figure 3-4 The UpdateSoftware Program.

3.3.5 Remote Data Retrieval

Using a computer running Flowlink and an appropriate cellular service, you can access your remote monitoring site in order to configure the flow module settings and retrieve flow data. Detailed instructions can be found in the Flowlink User Manual and Help files.

As a default Flowlink setting, the Quick Connect dialog box opens when you start Flowlink. To open Quick Connect manually, click the Quick Connect icon in the Flowlink toolbar. Then, click the DuraTracker button to connect. Flowlink will read the Dura-Tracker system information and attempt to match it with an existing site in the open database. If Flowlink cannot find a match for the connected site, it creates a new site within the database.

3.3.6 SMS	Using LTE technology and the appropriate SIM card, the Dura- Tracker is capable of sending digital text messages to up to five text-capable cellular devices when a pre-programmed alarm con- dition occurs. Consult the Flowlink User Manual and Help files for detailed information.				
	You can text "STATUS" to the unit's phone number and it will open up a 20 minute call window and send you its IP address. You can then use Flowlink to connect to the device remotely.				
3.3.7 Datapush	The DuraTracker can automatically send data to a designated server running ISCO Flowlink Pro software. The user-specified primary data transmission interval (5 minutes to 24 hours) can automatically change to a secondary interval when specific site conditions occur at the monitoring site. An Oracle® or Microsoft® SQL database is required to use this feature. Contact the factory for additional information.				
	To use the data push capability, connect to the DuraTracker and select the DATA tab. Click the PUSHED DATA button to set up a schedule for the data to be pushed to a Flowlink Pro server.				
	Image: State 220A03099 DT Goodyear2 052621 Image: State 208 17AM Connected Site: 220A03099 DT Goodyear2 052621 Jump to measurement tab >> 08 17AM Connected Site Info Devices Measurements Data 350 Level Alarms Wireless Power Control ADFM Modbus Input Modbus Dutput Modem TIE Net The top Isit box shows the storage locations while the bottom list box shows the measurements that are recording data. Data Storage Name Max Readings Utilization Oldes Reading Data Storage Fields S00 ISCO Area/Veolog Sensor -221E01959 Max Readings Utilization Oldest Reading Data Storage Fields				

D			011 10 1	D		
Data Storage Name 350 ISCO Area-Velocity Sensor - 221E01958	Max Read	ings Utilizati	on Oldest Reading	Data Sto	rage Fields	
DuraTracker						
Measurement	Primary	Secondary	Recent Reading	Readings	Quality	^
DuraTracker::Time			6/8/2021 8:16:30 AM	39059	100%	
DuraTracker::350 Level	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker:: 350 Velocity Signal	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker:: 350 Velocity Spectrum	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker:: 350 Vel Spectrum Ratio	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker::350 Temperature	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker::350 Sense Voltage	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker:: 350 Velocity	15 min	Off	6/8/2021 8:15:00 AM	1225	95%	
DuraTracker: Elow Bate	15 min	Off	6/8/2021 8:15:00 AM	1225	100%	~
Primary rate Push data every: 2 Hours			Synchronization			
Secondary rate	When		istrue Set E	quation	el 🦻 🏆	Help
Server Information P Listener Server IP address: 140.165.202.85		Server F	Port number: 1704			

Figure 3-5 Data tab

Detailed Flowlink instructions are beyond the scope of this manual. Flowlink's operating instructions are available in a Windows Help format. You can access the Help topics for an active window by clicking its HELP button or by pressing F1 on your computer's keyboard. You can also access Help topics by selecting HELP from the Flowlink menu.

3.3.8 Check connection

The connection to the server can be checked by running a manual data push. To start the manual data push, select the MODEM tab. You can change the amount of data to push by changing the START DATE/TIME and the END DATE/TIME. By default, these values are set to the 24-hour period of the current days date. Click START MANUAL DATA PUSH, and a window will appear that shows the connection. It will list each thing that it is doing and let you know if it fails along the way.

222C0	2472 Dura	Tracker Si	te													×
Site:			aTracker Sif	te			Ju	mp to me	asureme	int tab >>		08	5:44 AM -	Connected		
Site Info	Devices	Measure	ements Data	310 Dist	tance Alar	ms Wirele	ss Pow	er Control	ADFM	Modbus Inp	ut Modb	us Output	Modem	TIENet		
	-Inbound-															
		ct Connec	tion Mode:	P	•	Port:	1700		Serv	ice Provider:	Veriz	on	-	•		
	APN:		mw01.VZWS	TATIC		TCP Add	iress:	166.149	9.17.43							
	Usem	ame:				Phone nu	umber:	+15315	104033							
	Passw	vord:				Signal st	rength:	67 %								
	-Manual D	ata Push														
	🗲 Start D)ate:	4 /21/2022	•	12:00:00	AM 🗼					1					
_	🗲 End D	ate:	4 /21/2022	•	11:59:00	PM ÷		Star	t Manual	Data Push						
				_		_										
	Se	nd to Noti	lication Group:													
	SMS															
		trieval Inte	rval: 15	5 minutes	•											
Disc	connect (F2)		Retrieve Da	ta (F8)	DEFA	ULT Graph	(F3)	~	App	ly (F9)	X	Cancel		?	Help	
			C02472 D	T 1	<i>C</i> 1											
	ſ	Site:	C02472 Du			kar Cita						me to m		nent tab :		
				02472 D			Larar	D ¹ 1	1	lur i		-				.1
		Siteli	ito Device	s Meas	urements	Data	3101	Distanci	e Alar	ms Wirele	ss Pow	er Contro		м мос	ibus inpi	at Moi
			anual Data	Durch Charl					×	<u> </u>						
										Port	1700	_	Se	rvice Pro	vider.	Ver
			lanual Data ushing via:				06		^	TODALL	1	100.1	0 1 7 40			
			ate Range:	2022-04-1	21T00:00:	00 - 2022-	04-217	F23:59:0	0	TCP Add	ress:	166.14	19.17.43			
										Phone nu	mber:	+1531	510403:	3		
										Signal str	enath:	67 %				
										orginal ou	ongan.	00				
													$\mathbf{\setminus}$			
										M ÷						
												Ste	ut Manu	al Data F	Push	1
									\sim	M 📩						-
				<u>C</u> lear		<u>С</u> ору										

Figure 3-6 Manual Data Push

3.4 Configuration

3.4.1 Program Settings

The Site window of Flowlink contains all of the program settings that control the site's operation. The settings are entered within eight tabs as described in Table 3-1:

Table 3-1 Site	Window Tabs
Site Info	Basic Site Information
Devices	Connected Sensors
Measurements	Sensor Measurements
Data	Data Information
Alarms	Alarm Information
Wireless Power Control	Modem and Bluetooth Times
Modbus Input	Modbus Input Information
Modbus Output	Modbus Output Information
Modem	Modem Setup
TIENet	TIENet Sensor Setup

3.4.2 Site Name The DuraTracker is shipped with default names assigned to the unit so communication can immediately begin with Flowlink. To change the default site name, access the SITE INFO tab in Flowlink. The name must be unique among other site names already present in the Flowlink database.

Site names can be up to 20 characters long. Invalid characters include:

Table 3-2 Invalid Characters					
/	Forward slash				
\	Back slash				
:	Colon				
*	Asterisk				
?	Question mark				
"	Double-quote				
<	Left angle bracket				
>	Right angle bracket				
	Bar				
&	Ampersand				

3.4.3 Devices	TIENet devices that can be used are the 301pH and Temp sensor, 306 Sampler Interface, 310 Ex Ultrasonic sensor, 350 Area Velocity sensor, 350 Ex Area Velocity sensor, 360 LaserFlow velocity sensor, and 360 LaserFlow Ex velocity sensor.					
	Standard DuraTracker:					
	• The limit of 4 TIENet devices with any combination of 350, 310, 306, or 301, excluding the 360 LaserFlow.					
	• The limit of 360 LaserFlow sensors is 1, with a combi- nation of up to 3 other TIENet devices (350, 310, 306, or 301).					
	Note					
	360 LaserFlow battery banks will run in parallel at all times. It is recommended to use both banks of batteries when running a 360 LaserFlow.					
3.4.4 TIENet Setup	Selecting the TIENet tab will show what active TIENet devices are connected to the DuraTracker.					
Perform Scan	If TIENet devices have been added or removed from the system, Click on SCAN to detect the current system configuration.					
Sensor Differences	If there are any differences in the device configuration since the last scan, a list of Sensor Differences will appear.					
	Missing Sensors - The Missing Sensors list will indicate any previously connected devices that are no longer detected. Select Retain to keep the identification information for a previous device; select Remove to delete it.					
	Replaced Sensors - The Replaced Sensors list displays any newly added sensors that have replaced Missing Sensors that have been Retained.					
	Available TIENet Devices - Devices that are not currently con- figured show up here after a scan. Selecting a device and clicking on ADD will configure the device and moves it to the Active TIENet Devices window.					
Configure Active Parameters	Highlight the sensor in Active TIENet Devices window and click on CONFIGURE ACTIVE PARAMETERS to begin setting up mea- surement parameters for that TIENet device.					
	To activate a measurement, highlight the check box next to it and press OK.					

Configure TIENet Measurements		
-		
✓ 301 pH	301 Temperature	

Figure 3-7 301 pH and Temperature Sensor Parameters

Configure TIENet Measurements		
✓ 306 Sample Bottle	306 Input Voltage	

Figure 3-8 306 Sampler Interface Parameters

Configure TIENet Measurements		
Image: Transmission of the state of the	▼ 310 Level ▼ 310 Ultrasonic Signal	

Figure 3-9 310 Ex Ultrasonic Sensor Parameters

Configure TIENet Measurements		
✓ 350 Level ✓ 350 Velocity ✓ 350 Velocity Spectrum ✓ 350 Sense Voltage	350	Temperature Velocity Signal Vel Spectrum Ratio

Figure 3-10350 Ex Area Velocity Sensor Parameters

Confi	gure TIENet Measurements			
~	360 Distance	~	360 Level	
~	360 Velocity	~	360 Case Temperature	
	360 Laser Temperature	~	360 X-Axis	
~	360 Y-Axis	~	360 Laser Diode Current	
~	360 Ultrasonic Signal	~	360 Temperature	
~	360 Sense Voltage	~	360 Air Temperature	
	360 Doppler Power			

Figure 3-11360 LaserFlow Sensor Parameters

Configu	ure TIENet Measurements			
I	360 Distance	v	360 Level	
	360 Velocity	~	360 Case Temperature	
	360 Laser Temperature	~	360 X-Axis	
I	360 Y-Axis	~	360 Laser Diode Current	
I	360 Ultrasonic Signal	~	360 Temperature	
	360 Sense Voltage	•	360 Air Temperature	
	360 Input Voltage	•	360 Doppler Power	

Figure 3-12360 LaserFlow Ex Sensor Parameters

3.4.5 Data Storage Settings

Review the data storage settings within the DATA tab in Flowlink to ensure the pertinent types of data are being stored, and that the rate at which data is stored will provide a sufficient amount of data for your application.

The default data storage rate for the DuraTracker is set at once every 15 minutes for all readings except for total flow and input voltage readings which the default rate is once every 24 hours. You can modify the data storage rates to log readings more or less often.

🗹 Note

Although the DuraTracker can log data once every 15 seconds, increased data storage rates will shorten battery life, increase memory usage, and lengthen retrieve data (interrogation) times. Take this into consideration when making adjustments.

Data storage rates, as well as the types of data stored, can be modified within the Data Storage Setup Window as shown in Figure 3-13. This window can be accessed by selecting the SET UP DATA STORAGE button from the DATA or MEASUREMENT tabs.

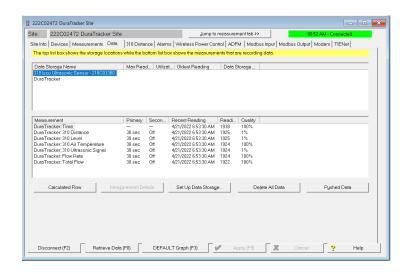


Figure 3-13 Data Storage Setup window

		Each measurement has a primary and secondary storage rate. The primary storage rate specifies the rate at which data is recorded under normal conditions. The secondary storage rate specifies the rate at which data is recorded when a user-defined condition exists. For example, the secondary storage rate can be set higher than the primary storage rate in order to respond to a rising water level. Using secondary storage rates will result in better resolution of data. The primary and secondary storage rates can be set to record data from once every 15 seconds to once every 24 hours. Alternatively, the primary and secondary storage rates can be turned off, and measurement readings will still occur but will not be recorded. This may be done if that mea- surement is used for calculations only.
3.4.6	Applying Setting Changes	After modifying a setting, click APPLY or press F9 on your com- puter's keyboard. Flowlink sends the change to the DuraTracker and updates the site's setting in its database.
3.4.7	Time Resolution	The time resolution for each measurement is one second. This means that measurements are taken at the same time as the time stamp. Measurements are not collected and averaged over a period of time prior to the time stamp.
3.4.8	Rollover Memory	The DuraTracker utilizes rollover memory to reduce data main- tenance. If memory becomes full, the DuraTracker overwrites the oldest measurement data with the newest measurement data. This occurs regardless of whether measurements are stored at the primary or secondary rate.

DuraTracker[®]

Section 4 Modbus Output Protocol

4.1 Overview Modbus is a simple command/response mechanism used to read from and write to specific digital memory locations known as registers. Modbus communication for the DuraTracker provides a standard protocol that can be used to retrieve real-time data from the DuraTrackers at a site, or multiple sites, over a wide area. The data can be sent to a central computer for display, collection, or process control. Modbus implementation is independent of Flowlink software and cannot alter the Flowlink programmed configuration of the DuraTracker. Modbus cannot be used to retrieve historical data from a DuraTracker's memory.

The DuraTracker utilizes Modbus ASCII and Modbus RTU protocols. Due to the wide variety of configurations that can be made with Modbus, it is impossible to cover every usable application within this user manual. Instead, this section outlines the basic capabilities and operations of Modbus output protocol as it applies to the DuraTracker. For this user manual, Modbus ASCII is discussed as it has more liberal communication timing requirements.

Commonly used terms related to Modbus output protocol are defined in Section 4.4.

To use Modbus Output on the DuraTracker, a jumper on the circuit board must be moved. This will allow Modbus output to be used but will result in higher battery consumption. Once the following has been completed, Modbus will be available to use.

1. Remove batteries from DuraTracker and open the front electronics panel by removing the six screws on the front of the unit. Before opening the case, make sure you are grounded so that you do not damage the internal components with an Electrostatic Discharge (ESD).

4.2 Setup



Figure 4-1 Screw removal

If case is opened to install a modem, change a SIM card or setup Modbus, ESD protection must be observed. Failing to do so could result in damage to the DuraTracker.

2. Open the case and disconnect the electrical connector and reference line from battery box.



Figure 4-2 Disconnecting electrical connector and reference line

3. Move Jumper J3 Modbus Power from the OFF position to the ON position.



Figure 4-3 Jumper position

4. Reconnect the electrical connector and reference line.

- 5. Line up the two halves of the case, being careful to make sure the wires from the electrical connector do not get pinched between the two halves.
- 6. Reattach the front panel with the screws removed in step 1.
 - a. Insert all of the previously removed screws into the holes. "Start" the screws to line up the threads of the screws to the threads of the hole. Do not fully tighten them until Step b.
 - When starting screws in plastic, you should always first turn them counterclockwise until you feel/hear the audible click of the threads lining up. Once the threads line up, you can then turn the screw clockwise to tighten it down. This will ensure that you do not cross-thread the plastic holes.
 - b. Tighten the screws in the sequence shown in Figure 4-4. This will ensure that the gaskets are tightened properly to maintain a watertight seal.
 - Repeat the sequence twice: first, tighten the screws enough to firmly hold the front half in place on the enclosure. Then, repeat the sequence to make the screws snug.

🗹 Note

Do not install screws using power tools. Use only hand tools.

Don't cross thread the screws. Always follow the tightening procedure above. Failure to tighten the screws correctly could result in water infiltration and damage to the DuraTracker.




Figure 4-4 Screw tightening sequence.

4.3 Operation

4.3.1	Establishing Communication	Several communications protocols supported in the DuraTracker series that require auto-baud rate detection. As a result, each time a Modbus connection is made, the module uses a polling mechanism to repeatedly send a command until a response is received. It may take up to 20 command retries before the unit has identified the baud rate and a response is received.
4.3.2	Module Addressing	When connecting to a site via a Modbus OPC server, use a dedi- cated line of communication to the DuraTracker from the OPC server. This can be a dedicated communications cable (direct con- nection) or a dedicated phone number (modem).
		While using a direction connection, you are dedicating a specified COM port on the computer. That COM port determines the site to which you are connecting.
		While using a modem, the dedicated line is defined by the site's phone number. If you connect more than one DuraTracker at a site, the Modbus OPC server must have some way of differenti- ating between the units. When sending a command to a specific unit, the command has an address field. This allows the server software to communicate with and control the specified unit while ignoring other units at that site.
4.3.3	Configurations	A variety of configurations can be created with Modbus though direct connection or through a modem.
		Figure 4-5 shows a direct connection between a server PC and a DuraTracker site using the COM ports on the OPC server. These COM ports are directly connected to the remote sites. Connection to the unit is made through the Power/Modbus communication port on the front of the DuraTracker.

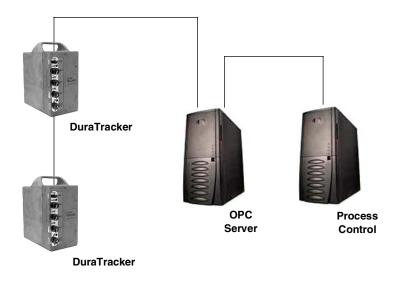


Figure 4-5 Configuration example

The operation sequence of the configuration shown in Figure 4-5 is as follows:

- 1. The DuraTrackers take readings from the probes.
- 2. The DuraTrackers store readings (level, velocity, flow rate, etc.) in their specified registers.
- 3. The user requests data through Process Control.
- 4. Process Control requests information from the OPC server.
- 5. The OPC server connects to the DuraTracker through the Power/Modbus port (direct connection), copies register data from the specified DuraTracker, and populates its holding index with this data.
- 6. Process Control retrieves the data from the OPC server's holding index and supplies the data to the user.

🗹 Note

Process Control can be activated manually or automatically in this example. The OPC server and Process Control may be physically located on the same computer.

4.4 Glossary of Terms

Table 4-1 defines terms commonly used with Modbus output protocol:

Table 4-1 M	odbus Terms
ASCII	American Standard Code for Infor- mation Interchange (ASCII) is a code that represents English char- acters with numbers. Most comput- ers represent characters with ASCII code. This makes it possible for one computer or device to share data with another. DuraTracker supports Modbus ASCII.
DCS	Distributed Control Systems.
Dedicated Line	A dedicated line is a telecommuni- cations path reserved for communi- cation between two specified points and not shared among multiple points.
Modbus Protocol	A Modbus protocol is a messaging structure used to establish mas- ter/slave server communications between intelligent devices. Mod- bus is a simple command/response mechanism to read from and write to registers.
MTU	Master Terminal Unit.
OPC	Object linking and embedding for Process Control (OPC) is a type of open connectivity which uses free-for-use standards. It is a series of software standards specifications that act as a translator for data transmission and process control. The specification defines a stan- dard set of objects, interfaces, and methods for use in process control and manufacturing automation appli- ances to facilitate interoperability.
PLC	Programmable Logic Controller.
Register	A register is a location in digital memory that have specific data stored for retrieval or for use with control functions. The definition of what information is contained and where (i.e., the registry number or address) is decided by the manufac- turer, Teledyne ISCO.
RTU	Remote Terminal Unit.

Table 4-1 M	odbus Terms
SCADA	A Supervisory Control And Data Acquisition (SCADA) is a computer system for gathering and analyzing real-time data. SCADA systems are used to monitor and control plant operation or equipment used in industries such as telecommunica- tions, water and wastewater control, energy, oil and gas refining, and transportation. The SCADA system transfers information to a central site, alerting the site of conditions, and performing necessary analysis and control. This information is dis- played in a logical and organized manner.
TCP/IP	Transmission Control Protocol/Internet Protocol.

4.5 DuraTracker ASCII or RTU Address	The DuraTracker's address (Device ID) is user programmable between 2 and 247.			
	Be careful not to assign the same address to more than one Logger.			
4.6 Register Definitions	The register definitions for the DuraTracker Logger are provided in the following table.			
	Where no other Unit Of Measure exists for a parameter, percent (%) can be used in most situations.			
4.6.1 Modbus Registers	Modbus tables are available through Flowlink.			

Register	Name	Data Type	Units of	Read/	Description
Number			Measure	Write	
40025	TakeReadingFlag	Word		R/W	Set to 1 to update readings, 2 for
					automatic update
40026	UpdateInterval	Word	Seconds	R/W	The reading update interval in
	-				seconds
40027	Activeflags	Word		R	The bit fields to indicate which
					sensors are active
40040	Level	Float	Meters	R	Level
40041					
40042	Levelstatus	Word		R	Non-zero is an error
40043 - 48	Leveltime	Word		R	The last level reading time,
					sec-min-hour-day-month-year
40055	Level1	Float	Meters	R	Level 1
40056					
40057	Level1status	Word		R	Non-zero is an error
40058 - 63	Level1time	Word		R	The last level 1 reading time,
					sec-min-hour-day-month-year
40070	Level2	Float	Meters	R	Level 2
40071					
40072	Level2status	Word		R	Non-zero is an error
40073 - 78	Level2time	Word		R	The last level 2 reading time,
					sec-min-hour-day-month-year
40085	Level3	Float	Meters	R	Level 3
40086					
40087	Level3status	Word		R	Non-zero is an error
40088 - 93	Level3time	Word		R	The last level 3 reading time,
					sec-min-hour-day-month-year
40100	Level4	Float	Meters	R	Level 4
40101					
40102	Level4status	Word		R	Non-zero is an error
40103 - 08	Level4time	Word		R	The last level 4 reading time,
					sec-min-hour-day-month-year
40115	Level5	Float	Meters	R	Level 5
40116					
40117	Level5status	Word		R	Non-zero is an error
40118 - 23	Level5time	Word		R	The last level 5 reading time,
					sec-min-hour-day-month-year
40130	Level6	Float	Meters	R	Level 6
40131					
40132	Level6status	Word		R	Non-zero is an error

Table C-1 Output Registers for DuraTracker Flowmeter

40133 - 38	Level6time	Word		R	The last level 6 reading time,
				_	sec-min-hour-day-month-year
40145	Level7	Float	Meters	R	Level 7
40146					
40157	Level7status	Word		R	Non-zero is an error
40158 - 63	Level7time	Word		R	The last level 7 reading time,
					sec-min-hour-day-month-year
40160	Velocity	Float	Meters/Sec	R	Velocity
40161					
40162	Velocitystatus	Word		R	Non-zero is an error
40163 - 68	Velocitytime	Word		R	The last velocity reading time,
					sec-min-hour-day-month-year
40175	Velocity1	Float	Meters/Sec	R	Velocity 1
40176					
40177	Velocity1status	Word		R	Non-zero is an error
40178 - 83	Velocity1time	Word		R	The last velocity 1 reading time,
					sec-min-hour-day-month-year
40190	Velocity2	Float	Meters/Sec	R	Velocity 2
40191					
40192	Velocity2status	Word		R	Non-zero is an error
40193 - 98	Velocity2time	Word		R	The last velocity 2 reading time,
					sec-min-hour-day-month-year
40205	Velocity3	Float	Meters/Sec	R	Velocity 3
40206					
40207	Velocity3status	Word		R	Non-zero is an error
40208 - 13	Velocity3time	Word		R	The last velocity 3 reading time,
					sec-min-hour-day-month-year
40220	Velocity4	Float	Meters/Sec	R	Velocity 4
40221					
40222	Velocity4status	Word		R	Non-zero is an error
40223 - 28	Velocity4time	Word		R	The last velocity 4 reading time,
					sec-min-hour-day-month-year
40235	Velocity5	Float	Meters/Sec	R	Velocity 5
40236					
40237	Velocity5status	Word		R	Non-zero is an error
40238 - 43	Velocity5time	Word		R	The last velocity 5 reading time,
	·				sec-min-hour-day-month-year
40250	Velocity6	Float	Meters/Sec	R	Velocity 6
40251					
40252	Velocity6status	Word		R	Non-zero is an error
40253 - 58	Velocity6time	Word		R	The last velocity 6 reading time,
	,				sec-min-hour-day-month-year
40265	Velocity7	Float	Meters/Sec	R	Velocity 7
40266	,		,		, ,

40267	Velocity7status	Word		R	Non-zero is an error
40268 - 73	Velocity7time	Word		R	The last velocity 7 reading time,
					sec-min-hour-day-month-year
40280	Flowrate	Float	Cubic	R	Flow rate
40281			Meters/Sec		
40282	Flowratestatus	Word		R	Non-zero is an error
40283 - 88	Flowratetime	Word		R	The last flow rate reading time,
					sec-min-hour-day-month-year
40295	Flowrate1	Float	Cubic	R	Flow rate 1
40296			Meters/Sec		
40297	Flowrate1status	Word		R	Non-zero is an error
40298 - 303	Flowrate1time	Word		R	The last flow rate 1 reading time,
					sec-min-hour-day-month-year
40310	Flowrate2	Float	Cubic	R	Flow rate 2
40311			Meters/Sec		
40312	Flowrate2status	Word		R	Non-zero is an error
40313 - 18	Flowrate2time	Word		R	The last flow rate 2 reading time,
					sec-min-hour-day-month-year
40325	Flowrate3	Float	Cubic	R	Flow rate 3
40326			Meters/Sec		
40327	Flowrate3status	Word		R	Non-zero is an error
40328 - 33	Flowrate3time	Word		R	The last flow rate 3 reading time,
					sec-min-hour-day-month-year
40340	Flowrate4	Float	Cubic	R	Flow rate 4
40341			Meters/Sec		
40342	Flowrate4status	Word		R	Non-zero is an error
40343 - 48	Flowrate4time	Word		R	The last flow rate 4 reading time,
					sec-min-hour-day-month-year
40355	Flowrate5	Float	Cubic	R	Flow rate 5
40356			Meters/Sec		
40357	Flowrate5status	Word		R	Non-zero is an error
40358 - 63	Flowrate5time	Word		R	The last flow rate 5 reading time,
					sec-min-hour-day-month-year
40370	Flowrate6	Float	Cubic	R	Flow rate 6
40371			Meters/Sec		
40372	Flowrate6status	Word		R	Non-zero is an error
40373 - 78	Flowrate6time	Word		R	The last flow rate 6 reading time,
					sec-min-hour-day-month-year
40385	Flowrate7	Float	Cubic	R	Flow rate 7
40386			Meters/Sec		
40387	Flowrate7status	Word		R	Non-zero is an error
40388 - 93	Flowrate7time	Word		R	The last flow rate 7 reading time,
					sec-min-hour-day-month-year

40400	Temperature	Float	Degrees	R	Temperature
40401			Celsius		
40402	Temperaturestatus	Word		R	Non-zero is an error
40403 - 08	Temperaturetime	Word		R	The last temperature reading
					time,
					sec-min-hour-day-month-year
40415	Temperature1	Float	Degrees	R	Temperature 1
40416			Celsius		
40417	Temperature1status	Word		R	Non-zero is an error
40418 - 23	Temperature1time	Word		R	The last temperature 1 reading
					time,
					sec-min-hour-day-month-year
40430	Temperature2	Float	Degrees	R	Temperature 2
40431			Celsius		
40432	Temperature2status	Word		R	Non-zero is an error
40433 - 38	Temperature2time	Word		R	The last temperature 2 reading
					time,
					sec-min-hour-day-month-year
40445	Temperature3	Float	Degrees	R	Temperature 3
40446			Celsius		
40447	Temperature3status	Word		R	Non-zero is an error
40448 - 53	Temperature3time	Word		R	The last temperature 3 reading
					time,
					sec-min-hour-day-month-year
40460	Volume	Float	Cubic	R	Volume
40461			Meters		
40462	Volumestatus	Word		R	Non-zero is an error
40463 - 68	Volumetime	Word		R	The last volume reading time,
					sec-min-hour-day-month-year
40475	Volume1	Float	Cubic	R	Volume 1
40476			Meters		
40477	Volume1status	Word		R	Non-zero is an error
40478 - 83	Volume1time	Word		R	The last volume 1 reading time,
					sec-min-hour-day-month-year
40490	Volume2	Float	Cubic	R	Volume 2
40491			Meters		
40492	Volume2status	Word		R	Non-zero is an error
40493 - 98	Volume2time	Word		R	The last volume 2 reading time
					sec-min-hour-day-month-year
40505	Volume3	Float	Cubic	R	Volume 3
40506			Meters		
40507	Volume3status	Word		R	Non-zero is an error
40508 - 13	Volume3time	Word		R	The last volume 3 reading time
					sec-min-hour-day-month-year

40520	Voltage	Float	Volts	R	Voltage
40521					
40522	Voltagestatus	Word		R	Non-zero is an error
40523 - 28	Voltagetime	Word		R	The last voltage reading time,
	-				sec-min-hour-day-month-year
40535	Voltage1	Float	Volts	R	Voltage 1
40536					
40537	Voltage1status	Word		R	Non-zero is an error
40538 - 43	Voltage1time	Word		R	The last voltage 1 reading time,
					sec-min-hour-day-month-year
40550	Voltage2	Float	Volts	R	Voltage 2
40551					
40552	Voltage2status	Word		R	Non-zero is an error
40553 - 58	Voltage2time	Word		R	The last voltage 2 reading time,
					sec-min-hour-day-month-year
40565	Voltage3	Float	Volts	R	Voltage 3
40566					
40567	Voltage3status	Word		R	Non-zero is an error
40568 - 73	Voltage3time	Word		R	The last voltage 3 reading time,
					sec-min-hour-day-month-year
40580	Analog/%	Float	4-20mA/	R	Analog output or percentage
40581			0-100%		
40582	Analog/status	Word		R	Non-zero is an error
40583 - 88	Analog/time	Word		R	The last Analog output or
					percentage reading time,
					sec-min-hour-day-month-year
40595	Analog/1	Float	4-20mA/	R	Analog output 1 or percentage
40596			0-100%		
40597	Analog/1status	Word		R	Non-zero is an error
40598 -608	Analog/1time	Word		R	The last Analog output 1 or
					percentage reading time,
					sec-min-hour-day-month-year
40610	Analog/2	Float	4-20mA/	R	Analog output 2 or percentage
40611			0-100%		
40612	Analog/2status	Word		R	Non-zero is an error
40613 -18	Analog/2time	Word		R	The last Analog output 2 or
					percentage reading time,
					sec-min-hour-day-month-year
40625	Analog/3	Float	4-20mA/	R	Analog output 3 or percentage
40626			0-100%		
40627	Analog/3status	Word		R	Non-zero is an error
40628 -33	Analog/3time	Word		R	The last Analog output 3 or
					percentage reading time,
					sec-min-hour-day-month-year

40640	Analog/4	Float	4-20mA/	R	Analog output 4 or percentage
40641			0-100%		
40642	Analog/4status	Word		R	Non-zero is an error
40643 -48	Analog/4time	Word		R	The last Analog output 4 or
					percentage reading time,
					sec-min-hour-day-month-year
40655	Analog/5	Float	4-20mA/	R	Analog output 5 or percentage
40656			0-100%		
40657	Analog/5status	Word		R	Non-zero is an error
40658 -63	Analog/5time	Word		R	The last Analog output 5 or
					percentage reading time,
					sec-min-hour-day-month-year
40670	Analog/6	Float	4-20mA/	R	Analog output 6 or percentage
40671			0-100%		
40672	Analog/6status	Word		R	Non-zero is an error
40673 -78	Analog/6time	Word		R	The last Analog output 6 or
					percentage reading time,
					sec-min-hour-day-month-year
40685	Analog/7	Float	4-20mA/	R	Analog output 7 or percentage
40686			0-100%		
40687	Analog/7status	Word		R	Non-zero is an error
40688 -93	Analog/7time	Word		R	The last Analog output 7 or
					percentage reading time,
					sec-min-hour-day-month-year
40700	Analog/8	Float	4-20mA/	R	Analog output 8 or percentage
40701			0-100%		
40702	Analog/8status	Word		R	Non-zero is an error
40703 -08	Analog/8time	Word		R	The last Analog output 8 or
					percentage reading time,
					sec-min-hour-day-month-year
40715	Analog/9	Float	4-20mA/	R	Analog output 9 or percentage
40716			0-100%		
40717	Analog/9status	Word		R	Non-zero is an error
40718 -23	Analog/9time	Word		R	The last Analog output 9 or
					percentage reading time,
					sec-min-hour-day-month-year
40730	Analog/10	Float	4-20mA/	R	Analog output 10 or percentage
40731	-		0-100%		
40732	Analog/10status	Word		R	Non-zero is an error
40733 -38	Analog/10time	Word		R	The last Analog output 10 or
					percentage reading time,
					sec-min-hour-day-month-year
40745	Analog/11	Float	4-20mA/	R	Analog output 11 or percentag
40746	<u> </u>		0-100%		

40747	Analog/11status	Word		R	Non-zero is an error
40748 -53	Analog/11time	Word		R	The last Analog output 11 or
					percentage reading time,
					sec-min-hour-day-month-year
40760	Analog/12	Float	4-20mA/	R	Analog output 12 or percentage
40761	Ċ.		0-100%		
40762	Analog/12status	Word		R	Non-zero is an error
40763 -68	Analog/12time	Word		R	The last Analog output 12 or
					percentage reading time,
					sec-min-hour-day-month-year
40775	Analog/13	Float	4-20mA/	R	Analog output 13 or percentage
40776	0,		0-100%		
40777	Analog/13status	Word		R	Non-zero is an error
40778 -83	Analog/13time	Word		R	The last Analog output 13 or
	0.				percentage reading time,
					sec-min-hour-day-month-year
40790	Analog/14	Float	4-20mA/	R	Analog output 14 or percentage
40791			0-100%		
40792	Analog/14status	Word	0 100/0	R	Non-zero is an error
40793 -98	Analog/14time	Word		R	The last Analog output 14 or
	0,				percentage reading time,
					sec-min-hour-day-month-year
40805	Analog/15	Float	4-20mA/	R	Analog output 15 or percentage
40806	0,		0-100%		
40807	Analog/15status	Word		R	Non-zero is an error
40808 -13	Analog/15time	Word		R	The last Analog output 15 or
					percentage reading time,
					sec-min-hour-day-month-year
40880	Fluoresence	Float	%	R	
40881					
40882	Fluoresencestatus	Word		R	
40883 - 88	Fluoresencetime	Word		R	
40895	Fluoresence1	Float	%	R	
40896					
40897	Fluoresence1status	Word		R	
40898 - 903	Fluoresence1time	Word		R	
40910	Fluoresence2	Float	%	R	
40911					
40912	Fluoresence2status	Word		R	
40913 - 18	Fluoresence2time	Word		R	
40925	Fluoresence3	Float	%	R	
40926					
40927	Fluoresence3status	Word		R	
40928 - 33	Fluoresence3time	Word		R	

40940	Battery	Float	Volts	R	
40941	Battery	Tioat	VOICS	N	
40941	Batterystatus	Word		R	
40943 - 48	Batterytime	Word		R	
40943 = 48	Battery1	Float	Volts	R	
	Datteryi	Tioat	VOICS	N	
40956 40957	Battery1status	Word		R	
40958 - 63	•	Word		R	
40938 - 63	Battery1time Battery2	Float	Volts	R	
	Datteryz	FIUAL	VOILS	n	
40971 40972	Patton/2status	Word		R	
40972	Battery2status	Word		R	
	Battery2time		Volta		
40985	Battery3	Float	Volts	R	
40986	Datta w 2atatua	14/aud			
40987	Battery3status	Word		R	
40988 - 93	Battery3time	Word		R	
41000	Dissolved Gas	Float	mmHg	R	
41001	.				
41002	Dissolved Gasstatus	Word		R	
41003 - 08	Dissolved Gastime	Word		R	
41015	Dissolved Gas1	Float	mmHg	R	
41016					
41017	Dissolved Gas1status	Word		R	
41018 - 23	Dissolved Gas1time	Word		R	
41030	Dissolved Gas2	Float	mmHg	R	
41031					
41032	Dissolved Gas2status	Word		R	
41033 - 38	Dissolved Gas2time	Word		R	
41045	Dissolved Gas3	Float	mmHg	R	
41046					
41047	Dissolved Gas3status	Word		R	
41048 - 53	Dissolved Gas3time	Word		R	
41120	Photosyn Rad	Float	umol s1 m2	R	
41121					
41122	Photosyn Radstatus	Word		R	
41123 - 28	Photosyn Radtime	Word		R	
41135	Photosyn Rad1	Float	umol s1 m2	R	
41136					
41137	Photosyn Rad1status	Word		R	
41138 - 43	Photosyn Rad1time	Word		R	
41150	Photosyn Rad2	Float	umol s1 m2	R	
41151					
41152	Photosyn Rad2status	Word		R	
41153 - 58	Photosyn Rad2time	Word		R	

41165	Photosyn Rad3	Float	umol s1 m2	R	1
	FIIOLOSYII NAUS	Fillat	unior si mz	n	
41166 41167	Photosyn Rad3status	Word		R	
41167	Photosyn Rad3time	Word		R	
41168 - 75	•	Float	%	R	
	Transmissivity	FIUal	70	ĸ	
41181	Tana and task it at at a	14/aud			
41182	Transmissivitystatus	Word		R	
41183 - 88	Transmissivitytime	Word	0(R	
41195	Transmissivity1	Float	%	R	
41196	— • • • • • • •				
41197	Transmissivity1status	Word		R	
41198 - 203	Transmissivity1time	Word		R	
41210	Transmissivity2	Float	%	R	
41211					
41212	Transmissivity2status	Word		R	
41213 - 18	Transmissivity2time	Word		R	
41225	Transmissivity3	Float	%	R	
41226					
41227	Transmissivity3status	Word		R	
41228 - 33	Transmissivity3time	Word		R	
41240	Conductivity	Float	uS/cm	R	
41241					
41242	Conductivitystatus	Word		R	
41243 - 48	Conductivitytime	Word		R	
41255	Conductivity1	Float	uS/cm	R	
41256					
41257	Conductivity1status	Word		R	
41258 - 63	Conductivity1time	Word		R	
41270	Conductivity2	Float	uS/cm	R	
41271					
41272	Conductivity2status	Word		R	
41273 - 78	Conductivity2time	Word		R	
41285	Conductivity3	Float	uS/cm	R	
41286					
41287	Conductivity3status	Word		R	
41288 - 93	Conductivity3time	Word		R	
41300	Specific Conductance	Float	uS/cm	R	
41301					
41302	Specific	Word		R	
	Conductancestatus				
41303 - 08	Specific	Word		R	
	Conductancetime				
41315	Specific Conductance1	Float	uS/cm	R	
41316					

	_				1
41317	Specific	Word		R	
	Conductance1status				
41318 - 23	Specific	Word		R	
	Conductance1time				
41330	Specific Conductance2	Float	uS/cm	R	
41331					
41332	Specific	Word		R	
	Conductance2status				
41333 - 38	Specific	Word		R	
	Conductance2time				
41345	Specific Conductance3	Float	uS/cm	R	
41346	•				
41347	Specific	Word		R	
	Conductance3status				
41348 - 53	Specific	Word		R	
	Conductance3time				
41360	Dissolved Solid	Float	mg/l	R	
41361		induc			
41362	Dissolved Solidstatus	Word		R	
41363 - 68	Dissolved Solidtime	Word		R	
41375	Dissolved Solid1	Float	mg/l	R	
	Dissolved Solidi	rioat	iiig/i		
41376 41377	Dissolved Solid1status	Word		R	
41378 - 83	Dissolved Solid1status	Word		R	
41378-83	Dissolved Solid1time Dissolved Solid2	Float	mg/l	R	
	Dissolved Solidz	FIUAL	iiig/i		
41391 41392	Dissolved Solid2status	Word		R	
41392	Dissolved Solid2status	Word		R	
41405	Dissolved Solid3	Float	mg/l	R	
41406	Disas kus d Calid 2status) A / a wal			
41407	Dissolved Solid3status	Word		R	
41408 - 13	Dissolved Solid3time	Word		R	
41420	Salinity	Float	mg/l	R	
41421					
41422	Salinitystatus	Word		R	
41423 - 28	Salinitytime	Word		R	
41435	Salinity1	Float	mg/l	R	
41436					
41437	Salinity1status	Word		R	
41438 - 43	Salinity1time	Word		R	
41450	Salinity2	Float	mg/l	R	
41451					
41452	Salinity2status	Word		R	
41453 - 58	Salinity2time	Word		R	

41465	Salinity3	Float	mg/l	R	
41466			C.		
41467	Salinity3status	Word		R	
41468 - 73	Salinity3time	Word		R	
41480	Dissolved Oxygen	Float	mg/l	R	
41481	10		0,		
41482	Dissolved Oxygenstatus	Word		R	
	,0				
41483 - 88	Dissolved Oxygentime	Word		R	
41495	Dissolved Oxygen1	Float	mg/l	R	
41496			_		
41497	Dissolved Oxygen1status	Word		R	
41498 - 503	Dissolved Oxygen1time	Word		R	
41510	Dissolved Oxygen2	Float	mg/l	R	
41511					
41512	Dissolved Oxygen2status	Word		R	
41513 - 18	Dissolved Oxygen2time	Word		R	
41525	Dissolved Oxygen3	Float	mg/l	R	
41526					
41527	Dissolved Oxygen3status	Word		R	
41528 - 33	Dissolved Oxygen3time	Word		R	
41540	рН	Float	рН	R	
41541					
41542	pHstatus	Word		R	
41543 - 48	pHtime	Word		R	
41555	pH1	Float	рН	R	
41556					
41557	pH1status	Word		R	
41558 - 63	pH1time	Word		R	
41570	pH2	Float	рН	R	
41571					
41572	pH2status	Word		R	
41573 - 78	pH2time	Word		R	
41585	pH3	Float	рН	R	
41586					
41587	pH3status	Word		R	
41588 - 93	pH3time	Word		R	

		I			1
41600	ORP	Float	Volts	R	
41601					
41602	ORPstatus	Word		R	
41603 - 08	ORPtime	Word		R	
41615	ORP1	Float	Volts	R	
41616					
41617	ORP1status	Word		R	
41618 - 23	ORP1time	Word		R	
41630	ORP2	Float	Volts	R	
41631					
41632	ORP2status	Word		R	
41633 - 38	ORP2time	Word		R	
41645	ORP3	Float	Volts	R	
41646					
41647	ORP3status	Word		R	
41648 - 53	ORP3time	Word		R	
41660	NH4 Nitrogen	Float	mg/l	R	
41661					
41662	NH4 Nitrogenstatus	Word		R	
41663 - 68	NH4 Nitrogentime	Word		R	
41675	NH4 Nitrogen1	Float	mg/l	R	
41676	_		-		
41677	NH4 Nitrogen1status	Word		R	
41678 - 83	NH4 Nitrogen1time	Word		R	
41690	NH4 Nitrogen2	Float	mg/l	R	
41691			-		
41692	NH4 Nitrogen2status	Word		R	
41693 - 98	NH4 Nitrogen2time	Word		R	
41705	NH4 Nitrogen3	Float	mg/l	R	
41706	Ū		0.		
41707	NH4 Nitrogen3status	Word		R	
41708 - 13	NH4 Nitrogen3time	Word		R	
41720	NO3 Nitrogen	Float	mg/l	R	
41721	Ū		0.		
41722	NO3 Nitrogenstatus	Word		R	
41723 - 28	NO3 Nitrogentime	Word		R	
41735	NO3 Nitrogen1	Float	mg/l	R	
41736			07.		
41737	NO3 Nitrogen1status	Word		R	
41738 - 43	NO3 Nitrogen1time	Word		R	
41750	NO3 Nitrogen2	Float	mg/l	R	
41751					
41752	NO3 Nitrogen2status	Word		R	
41753 - 58	NO3 Nitrogen2time	Word		R	
-11,22 - 20	NOS NILI OBELIZIIIIE	woru		N	

41765	NO3 Nitrogen3	Float	mg/l	R	
41766					
41767	NO3 Nitrogen3status	Word		R	
41768 - 73	NO3 Nitrogen3time	Word		R	
41780	Turbidity	Float	NTU	R	
41781					
41782	Turbiditystatus	Word		R	
41783 - 88	Turbiditytime	Word		R	
41795	Turbidity1	Float	NTU	R	
41796					
41797	Turbidity1status	Word		R	
41798 - 803	Turbidity1time	Word		R	
41810	Turbidity2	Float	NTU	R	
41811					
41812	Turbidity2status	Word		R	
41813 - 18	Turbidity2time	Word		R	
41825	Turbidity3	Float	NTU	R	
41826					
41827	Turbidity3status	Word		R	
41828 - 33	Turbidity3time	Word		R	
41840	Chloride	Float	mg/l	R	
41841					
41842	Chloridestatus	Word		R	
41843 - 48	Chloridetime	Word		R	
41855	Chloride1	Float	mg/l	R	
41856					
41857	Chloride1status	Word		R	
41858 - 63	Chloride1time	Word		R	
41870	Chloride2	Float	mg/l	R	
41871			0.		
41872	Chloride2status	Word		R	
41873 - 78	Chloride2time	Word		R	
41885	Chloride3	Float	mg/l	R	
41886			0,		
41887	Chloride3status	Word		R	
41888 - 93	Chloride3time	Word		R	
41900	Resistivity	Float	Ohm-cm	R	
41901					
41902	Resistivitystatus	Word		R	
41903 - 08	Resistivitytime	Word		R	
41915	Resistivity1	Float	Ohm-cm	R	
41916	Neolocivity 1	1.000			
41918	Resistivity1status	Word		R	
41918 - 23	Resistivity1time	Word	+	R	
41910-23	NESISUVILYLIIIIE	woru		n	

41930	Resistivity2	Float	Ohm-cm	R	
41931					
41932	Resistivity2status	Word		R	
41933 - 38	Resistivity2time	Word		R	
41945	Resistivity3	Float	Ohm-cm	R	
41946					
41947	Resistivity3status	Word		R	
41948 - 53	Resistivity3time	Word		R	
41960	Pressure	Float	mmHg	R	
41961	i i coodi c	liout			
41962	Pressurestatus	Word		R	
41963 - 68	Pressuretime	Word		R	
41975	Pressure1	Float	mmHg	R	
41976	1100001012	liout			
41977	Pressure1status	Word		R	
41978 - 83	Pressure1time	Word		R	
41990	Pressure2	Float	mmHg	R	
41991	110000102	liout			
41992	Pressure2status	Word		R	
41993 - 98	Pressure2time	Word		R	
42005	Pressure3	Float	mmHg	R	
42005	110350105	Tiout			
42007		Word		R	
42008 - 13	Pressure3time	Word		R	
42020	Reserved	Float		R	
42020	Reserved	liout		, N	
42021	Reservedstatus	Word		R	
42023 - 28	Reservedtime	Word		R	
42035	Generic	Float		R	
42036	Generie	liout		, N	
42030	Genericstatus	Word		R	
42038 - 43	Generictime	Word		R	
42050	Generic1	Float		R	
42051	Generioz	liout			
42052	Generic1status	Word		R	
42053 - 58	Generic1time	Word		R	
42065	Generic2	Float		R	
42066					
42067	Generic2status	Word		R	
42068 - 73	Generic2time	Word		R	
42080	Generic3	Float		R	
42080					
42081	Generic3status	Word		R	
			1		1

42095	Generic4	Float	R	
42096				
42097	Generic4status	Word	R	
42098 - 103	Generic4time	Word	R	
42110	Generic5	Float	R	
42111				
42112	Generic5status	Word	R	
42113 - 18	Generic5time	Word	R	
42125	Generic6	Float	R	
42126				
42127	Generic6status	Word	R	
42128 - 33	Generic6time	Word	R	
42140	Generic7	Float	R	
42141				
42142	Generic7status	Word	R	
42143 - 48	Generic7time	Word	R	
42155	Generic8	Float	R	
42156				
42157	Generic8status	Word	R	
42158 - 63	Generic8time	Word	R	
42170	Wireless Power	Float	R	
42171				
42172	Wireless Powerstatus	Word	R	
42172 - 78	Wireless Powertime	Word	R	
42185	Wireless Power1	Float	R	
42186				
42187	Wireless Power1status	Word	R	
42188 - 93	Wireless Power1time	Word	R	
42200	Wireless Power2	Float	R	
42201				
42202	Wireless Power2status	Word	R	
42203 - 08	Wireless Power2time	Word	R	
42215	Wireless Power3	Float	R	
42216	·····			
42217	Wireless Power3status	Word	R	
42242 22				
42218 - 23	Wireless Power3time	Word	R	
42230	Wireless Power4	Float	R	
42231	M/malaas Da			
42232	Wireless Power4status	Word	R	
42233 - 38	Wireless Power4time	Word	R	

42245	Wireless Power5	Float	R	
42246				
42247	Wireless Power5status	Word	R	
42248 - 53	Wireless Power5time	Word	R	
42260	Wireless Power6	Float	R	
42261				
42262	Wireless Power6status	Word	R	
42263 - 68	Wireless Power6time	Word	R	
42275	Wireless Power7	Float	R	
42276				
42277	Wireless Power7status	Word	R	
42278 - 83	Wireless Power7time	Word	R	
42290	Humidity	Float	R	
42291				
42292	Humiditystatus	Word	R	
42293 - 98	Humiditytime	Word	R	
42305	Humidity1	Float	R	
42306				
42307	Humidity1status	Word	R	
42308 - 13	Humidity1time	Word	R	
42320	Humidity2	Float	R	
42321				
42322	Humidity2status	Word	R	
42323 - 28	Humidity2time	Word	R	
42335	Humidity3	Float	R	
42336				
42337	Humidity3status	Word	R	
42338 - 43	Humidity3time	Word	R	
42350	Angle	Float	R	
42351				
42352	Anglestatus	Word	R	
42353 - 58	Angletime	Word	R	
42365	Angle1	Float	R	
42366				
42367	Angle1status	Word	R	
42368 - 73	Angle1time	Word	R	
42380	Angle2	Float	R	
42381	-			
42382	Angle2status	Word	R	
42383 - 88	Angle2time	Word	R	

42395	Angle3	Float	R	
42396				
42397	Angle3status	Word	R	
42398 - 403	Angle3time	Word	R	

DuraTracker®

Section 5 Maintenance

5.1 Overview	This section describes the maintenance requirements of the DuraTracker. The DuraTracker flow meter is designed to perform reliably in adverse conditions with a minimal amount of routine service. To keep your system working properly, the battery power and desiccant condition should be checked at regular intervals.				
	 Maintenance intervals are affected by many variables. For example, the number of sensors and the data storage rate will affect the battery life. Additionally, humidity levels affect the service life of the desiccant. Generally, a basic system installed in an environment with moderate humidity levels should function well with maintenance intervals under three months. A weekly maintenance interval is recommended until an understanding of the DuraTracker's operational capabilities under differing environmental conditions is gained. 				
	If the case is opened to install a modem, change a SIM card, or set up Modbus, ESD protection must be observed. Failing to do so could result in damage to the DuraTracker.				
5.2 Maintenance Kits	The maintenance kit for the DuraTracker contains O-rings for the connectors and desiccant cartridge, two hydrophobic filters, a one-pound container of indicating silica gel desiccant, a container of lubricant, and gaskets for the battery and desiccant caps. You can order maintenance kits by contacting Teledyne ISCO's WEB store (https://store.teledyneisco.com/). Contact information for Teledyne ISCO's Customer Service Department can be found in Appendix A.3.1.				
5.3 Battery Maintenance	Input voltage can be monitored while you are connected to the DuraTracker through Flowlink. The DuraTracker can also record input voltage readings to closely track power consumption. Battery discharge rates vary widely depending on the system's configuration and its operating environment. Batteries should be replaced according to the instructions in Section 2.6.				
	Primary cell or non-rechargeable batteries should always be replaced with new batteries.				
	The DuraTracker uses a CR2032 Lithium coin cell battery for backup. This battery should be replaced every 10 years.				
5.3.1 Battery Usage	The DuraTracker unit is equipped with two battery banks; however, it can operate using a single bank.				

☑ Note

A 360 Laserflow will always use the battery banks in parallel.


Generally, when both battery banks are installed, the unit uses them in parallel when they both have either a high (>12.3 volts) or a low (<9.4 volts) state of charge (SoC). Otherwise, the unit uses only one of the banks.

A power cycle at any time will cause the DuraTracker unit to switch to the battery bank with the highest remaining voltage.

A DuraTracker unit switches between parallel and single-bank battery usage to extend battery life while providing itself with adequate power. For example, the unit will switch to parallel bank usage whenever it detects a high SoC in both battery banks, because that behavior will reduce battery losses from self-discharge over time.

Understanding the DuraTracker unit's battery bank switching behavior can help you better decide when to replace its batteries.


1. In this example, both battery banks have a high SoC (>12.3 V), so they run together in parallel at first.



5.3.2 Battery Usage Examples

Fully-charged battery banks running in parallel.


2. Battery bank 1 has dropped below the high SoC.¹ At that point, the DuraTracker begins to use a single battery bank. In this example, it uses bank 2 because that is the one with the highest remaining voltage. (Bank 1 would have been chosen instead if it had the higher voltage.)

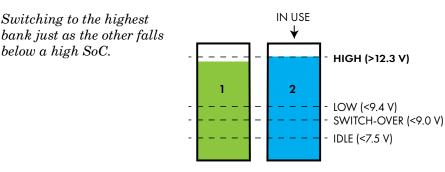

Switching to the highest


below a high SoC.

3. The DuraTracker will continue to run from that single battery bank until its voltage falls below the switch-over threshold (<9.0 V).

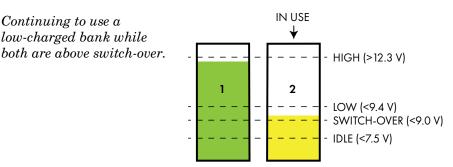


^{1.} Actually, with the exception of idle mode, each battery threshold has a total hysteresis of 0.20 volts. For example, at the high state of charge threshold, battery switching occurs between 12.4 volts and 12.2 volts. This behavior prevents frequent battery banks switching, thus improving battery life.

the other is below the switch-over threshold. 4. Battery bank 2 has fallen below the switch-over threshold. At this point, the DuraTracker unit detects that battery bank 1 has a higher remaining charge, so it switches to that bank.

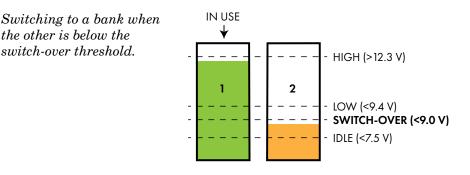



5. Battery bank 2 is replaced. But even though bank 2 has the highest SoC, the DuraTracker unit continues to run from bank 1. It will continue to do so until bank 1 reaches the switch-over threshold.

Adding a fresh battery bank while the other is above the switch-over threshold




6. Bank 1 has reached the low SoC threshold (9.4 V). If battery bank 2 was not replaced (as shown in the previous instance), it is well below the low SoC. With both banks low, the DuraTracker unit returns to parallel mode.






7. Possibly, battery bank 1 is replaced with a fresh bank that is above the low SoC threshold. In this case, the Dura-Tracker unit uses only bank 1 until it too falls below the switch-over threshold. (Compare to example 5, where *both* banks are still above that threshold.)




8. Or, possibly, neither battery is replaced, and both voltages drop below the switch-over threshold (9.0 V). The Dura-Tracker unit then enters Limp mode, as explained below.




Switching to a fresh battery bank when the

switch-over threshold.

other is below the



9. Eventually, both voltages drop could below the idle threshold (7.5 V). The DuraTracker unit then enters Idle mode, as explained below.



Limp mode. When both battery bank voltages drop below the 9.0 V (9.2 v in single batter bank) switch-over threshold, the DuraTracker unit will enter Limp mode, in which modem and Bluetooth functions are unavailable.

Running battery banks parallel in Idle mode.

Idle mode. When both battery bank voltages drop below the 7.5 V, idle threshold, the DuraTracker unit will enter Idle mode. At that point, the DuraTracker ceases all functions and enters an extended low-power sleep mode, only waking up to check the battery bank voltages once a minute. The DuraTracker will only return to normal operation if at least one battery bank voltage is detected to exceed the low state of charge threshold.

5.4 Surcharging Precaution If the DuraTrackers enclosure has been opened, ensure that the six screws that hold the front panel are tight before installing the unit. If they are not, follow the screw-tightening procedure described in Section 2.2.1 and Section 4.2 to ensure a watertight seal in the event of surcharging.

Leaving front panel screws loose could result in water infiltration and damage to the DuraTracker.

5.5 Desiccant Maintenance The DuraTracker uses desiccant to protect the internal components of the device from moisture damage. Each DuraTracker utilizes two desiccant cartridges, as shown in Figure 5-1.

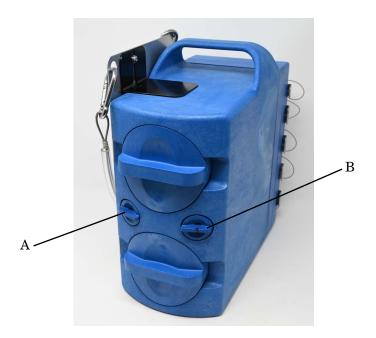


Figure 5-1 Desiccant cartridge locations

The desiccant cartridge "A" is used to remove moisture from the reference air utilized by the sensor and electronics box. This prevents moisture from plugging the reference line, which would result in the sensor reporting erroneous level readings. The desiccant cartridge "B" is used to remove moisture from the battery box.

The cartridges are filled with silica gel beads that will indicate when they are saturated. Under dry conditions, the beads are orange in color. As the desiccant becomes saturated, the beads turn green. If the entire length of the desiccant cartridge turns green, the unit is no longer adequately protected. Replace the desiccant before the entire length of the desiccant cartridge turns green.

5.5.1 Replacing Desiccant The desiccant is contained within the cartridge located between the battery banks. To remove the cartridge, unscrew the cap 1/4 turn counter-clockwise, and slide the cartridge out of the unit. The clear tube reveals the silica gel desiccant inside. To replace the desiccant:

- 1. Hold the cartridge upright with the cap at the top.
- 2. Push the cap off of the cartridge with thumb.

Figure 5-2 Removal of Desiccant Cartridge Cap

- 3. Empty the saturated silica gel desiccant beads or granules into a separate container.
 - a. For instructions on how to reactivate saturated silica gel desiccant, see Section 5.5.2.
- 4. Fill the tube with new or reactivated silica gel desiccant.
- 5. Press the cap back onto the cartridge.
- 6. Slide the cartridge into the DuraTracker battery compartment, and tighten the cap 1/4 clockwise to seal the cartridge in place.

5.5.2 Reactivating Desiccant Once saturated, silica gel desiccant can no longer suitably protect the DuraTracker from moisture. The silica gel desiccant can be reactivated as described below:

1. Pour the saturated silica gel desiccant into a heat resistant container.

Do not heat the silica gel desiccant cartridge assembly. It will melt.



- 2. Heat the desiccant in a vented convection oven at 212 to 350° F (100 to 175° C) for two to three hours, or until the orange color returns.
- 3. Remove the desiccant from the oven and allow it to cool.
- 4. Store the reactivated desiccant in an air-tight container until it is ready for use.

It has been reported that the silica gel desiccant may produce irritating fumes when heated. Although Teledyne ISCO has not been able to reproduce these reports, it is recommended that you always reactivate desiccant in a well-ventilated room and use the recommended temperature range. As an added precaution, it is recommended that you leave the room while the reactivation process takes place.

🗹 Note

The silica gel desiccant may lose its ability to remove moisture after several reactivations. This may result in more frequent maintenance requirements. If the desiccant becomes ineffective, replace it with new desiccant.

The DuraTracker is equipped with a hydrophobic filter which blocks water from the desiccant cartridge if the DuraTracker is subjected to extremely humid or submerged conditions. Any amount of liquid water will plug the filter and restrict access to sensitive components. If this occurs, the filter must be removed, rinsed with clean water, and allowed to dry. Alternatively, the filter may need to be replaced.

To remove the hydrophobic filter, use a 5/8" or 16 mm socket wrench to gently unscrew the filter from the DuraTracker. Then, gently screw the replacement filter into place.



Figure 5-3 Replacing the hydrophobic filter

If the hydrophobic filter requires frequent replacement, consider relocating the unit to an area that is more suitably protected.

5.6 Hydrophobic Filter Maintenance

Note

Unsteady TIENet 350 AV Level sensor reading are often an indication that the hydrophobic filter may be plugged.

5.7 Cleaning the DuraTracker	Before cleaning the module, ensure that all protective connector caps are in place. The housing of the DuraTracker should be cleaned with a mild detergent and warm water.
	The cables and outer surfaces of the TIENet sensors may also be cleaned with a mild detergent and warm water.
5.8 Servicing the DuraTracker	The internal components of the DuraTracker are not user-ser- viceable. If the DuraTracker requires repair, contact Teledyne ISCO's Water Product support. Contact information for- Teledyne ISCO can be found in Appendix A.3.1.
	Corresponding with a Teledyne ISCO technical service represen- tative often resolves problems with the unit without the need to return the item. If the problem cannot be resolved, you will be issued a Return Merchandise Authorization (RMA) and instruc- tions on how to return the unit to the factory.
5.9 Diagnostics	Many functions of the DuraTracker generate a diagnostic file. Diagnostic files can often be used to isolate a problem so it can be adequately understood and fixed.
	To view a diagnostic file, connect to the site using Flowlink. Within the MEASUREMENT tab of the problematic function, click the DIAGNOSTICS button. This prompts the DuraTracker to gen- erate a diagnostic file which is accessed by Flowlink as a text report.

ite:	222C024	472 DuraTri	acker Site	e		J	ump to measu	rement tab >>		07:01 AM	/- Connecte	ł k
Site Info	Devices	Measuremen	ts Data	310 Level	Alerms Wi	reless Power	Control ADFN	/ Modbus Input	Modbus C	utput Modem	TIENet	
Setup	the measur	ement								Set Up Da	ata Storage	
	Meas	Module nam surement nam Measureme	e: 310 Lex		feet		•		Г	Diag Hide in Measu	nostics	
Blanking I N Resourc Pre- (Check measur	this box for Al	4/20/2022 2	R R R surements the	h								

Figure 5-4 Retrieving diagnostic files manually

Diagnostic files can also be retrieved while Flowlink retrieves site data. The most recent diagnostic files are kept in Flowlink's database where they can be accessed at a later date. To enable this feature, open UTILITIES > OPTIONS from the menu and check "Retrieve data gets text reports" on the DuraTracker tab.

	aTracker Site		
Site: 222C0:	2472 DuraTracker Site	Jump to measurement tab >> 06:59 AM - Co	innected
Site Info Devices	Measurements Data 310 Distance Alarms Wire	less Power Control ADFM Modbus Input Modbus Output Modem	TIENet
The top list box	hour the stars a location while the better list how shows Options	the measurements that are recording data	×
Data Storage N 310 Isco Ultras; DuraTracker: DuraTracker: DuraTracker:3 DuraTracker:3 DuraTracker:3 DuraTracker:7 DuraTracker:7		Wizard Pulse Doppler Default Units Graph Defaults Misc eries of instruments. C TCP C Default to 2100/Dura Tracker Baud rate: 115200 V Port 1700	
Calculat	Retrieve data gets text reports Display communication statistics Show connection dialog on startup	Parameters	
		OK Cancel ? H	elp
Disconnect (Fi	2) Retrieve Data (F8) DEFAULT Grap	oh (F3) 🖌 Apply (F9) 🗮 Cancel 🧕 🤋	Help

Figure 5-5 Retrieving diagnostic files automatically

DuraTracker®

Appendix A

A.1 Replacement Parts

A.2 Optional Equipment and Accessories

Ordering Information

Options and accessories can be purchased by visiting the Teledyne ISCO online store at <u>store.teledyneisco.com</u>.

DuraTracker Logger Accessories

A.2.1 Cables and Accesories

USB communication cable (6ft)	480 - 2946 - 06
Power/Modbus communication cable (25ft)	60-4804-023
Din rail mount DC power supply, Input 115-230 VAC 50/60 Hz, Output 12 VDC 1.5A	340-0002-18
TIENet Cable with TIENet plug on one side cut to length	60-4804-071
Silica gel desiccant, 1.0-lb container	60-2004-233
DuraTracker maintenance kit	60-4804-021
TIENet 'Y' connection cable	60-4304-066
TIENet Expansion Box w/ 10 ft cable	60-4307-023
TIENet Expansion Box w/ 10 ft cable and reference air support	60-4357-018
Ex Reference Air Box w/ 10m cable	68-4800-025
Ex Reference Air Box w/ 23m cable	68-4800-026
Ex Reference Air Box w/ cut to length cable	68-4800-027
Spreader bar for suspension of sensor or flow meter in manhole shaft	60-3004-110

A.2.2 Battery Options

Spiral wound Lithium Thionyl Chloride D cell battery (low temp applications)	340-9036-00
Lithium Thionyl Chloride battery holder (DuraTracker ONLY)	60-4804-026
Lantern battery holder (DuraTracker ONLY)	60-4804-025
Hazloc D cell battery holder	60-4804-024

A.2.3 301 pH/Temperatu	The Includes combination pH probe with built-in exposed temperature
Device Ending in	probe and 25 ft. probe cable and one package of each buffer and
TIENet Plug	rinse solution for probe calibration
10 m cable [*]	
23 m cable*	
Cut-to-length cable*	
0	* Cable lengths from Signature to TIFNet 201 device

* Cable lengths from Signature to TIENet 301 device

A.2.4 306 Sampler Interface Cable with Connection Ending in TIENet Plug

306 Sampler Interface w/ connector and 10m (32.8 ft) cable	60-4304-076
306 Sampler Interface w/ connector and 23 m (75 ft) cable	$\dots 60-4304-077$
306 Sampler Interface w/ connector and CTL cable	$\dots 60-4304-078$

A.2.5 310 Ex Ultrasonic Level Sensor with Connection Ending in TIENet Plug

009
)11
11
)13
)

A.2.6 360 LaserFlow Velocity Sensor with Connection Ending in TIENet Plug

360 Laserflow sensor w/ connector and 10m cable	
360 Laserflow sensor w/ connector and 23m cable	
360 Laserflow sensor w/ connector Cut-to-length*	
* Cable lengths can go up to 15	0 m
360 Laserflow sensor w/ connector and 10m cable +USNC	

360 Laserflow sensor w/ connector and 23m cable +USNC	8-2160-061 – ISCO3101
360 Laserflow sensor w/ connector Cut-to-length* +USNC	

 * Cable lengths can go up to 150 m $\,$

A.2.7 360 LaserFlow Ex Velocity Sensor with Connection Ending in TIENet Plug

360 Laserflow Ex sensor w/ connector and 10m cable	60-4364-095
360 Laserflow Ex sensor w/ connector and 23m cable	60-4364-098
360 Laserflow Ex sensor w/ connector Cut-to-length*	60-4364-099
* Cable lengths can go up to 33 m	

360 Laserflow Ex sensor w/ connector and 10m cable +USNC	
360 Laserflow Ex sensor w/ connector and 23m cable +USNC	
360 Laserflow Ex sensor w/ connector Cut-to-length* +USNC	60-4364-105
* Cable lengths can go up to 33 m	

A.2.8 350 Ex Area Velocity Sensor with Connection Ending in TIENet Plug

350 Ex Area Velocity Surcharge sensor	
350 Ex Area Velocity sensor with connector and 10m cable	
350 Ex Area Velocity sensor with connector and 23m cable	
350 Ex Area Velocity sensor with connector Cut-to-length*	
* Cable lengths can go up to 30 m	

A.2.9 Modems

DuraTracker (cannot be used in DuraTracker Ex)

A.3 Company Contact Information

A.3.1 Customer Service	Teledyne ISCO
Department	Technical Service Dept.
	4700 Superior Street
	Lincoln, NE 68504 USA

Phone: (866) 298-6174 (402) 464-0231

FAX:(402) 465-3022

E-mail: iscowatersupport@teledyne.com

DuraTracker[®] Appendix A

DuraTracker®

Appendix B Material Safety Data Sheets

B.1 Safety

This appendix provides Material Safety Data Sheets for the desiccant used by the DuraTracker Logger.

Teledyne ISCO cannot guarantee the accuracy of the data. Specific questions regarding the use and handling of the products should be directed to the manufacturer listed on the MSDS.

 $\operatorname{SORB-IT}^{\circledast}$ is a registered trademark of N. T. Gates Company.





sSORB®



Product Name: sSOI Chemical Name: Yel	B [®] ow Indicating Silica Gel	Supplier:	Interra Global 371 Edgemon	
Synonyms: Orange Indicating Silica Gel			Park Ridge, IL	60068
			USA	
Emergency Assistan	ce			
USA	+ 1.847.292.8600		Telephone:	+ 1.847.292.8600
Outside USA	+ 1.847.292.8600		Fax:	+ 1.847.292.8601

Section 2: COMPOSITION & INFORMATION ON INGREDIENTS

CAS Numbers: 1343-98-2, 77-09-8

Molecular Formula: SiO₂ · nH₂O + C₂₀H₁₄O₄

Section 3: HAZARDS IDENTIFICATION

Potential Health Effects

Inhalation: May cause dryness and irritation to mucous membranes, nose and throat. Symptoms may include coughing, sore throat, and wheezing.

Ingestion: No adverse effects expected.

Skin Contact: May cause irritation with dryness and abrasion.

Eye Contact: May cause irritation, redness and pain.

Chronic Exposure: Repeated exposure may cause symptoms similar to those listed for acute effects. Synthetic amorphous silica does not produce silicosis.

Section 4: FIRST AID MEASURES

Eye Contact: Check for and remove any contact lenses. In case of contact, immediately flush eyes wth plenty of water for at least 15 minutes. Get medical attention if irritation occurs.

Skin Contact: Wash with soap and water. Cover the irritated skin with an emollient. Get medical attention if irritation develops.

Ingestion: Give several glasses of water to drink to dilute. If large amounts were swallowed, get medical advice.

Inhalation: If inhaled, remove to fresh air. If breathing is difficult, get medical attention.

Section 5: FIRE & EXPLOSION DATA

Fire: Not considered to be a fire hazard.

Explosion: Not considered to be an explosion hazard.

Fire Fighting Media and Instructions: Use any means suitable for extinguishing surronding fire.

Special Remarks: Use protective clothing and breathing equipment appropriate for surronding fire.

INTERRA Global Corporation

msds sSORB

p1

SEP 2 1 2012

MATERIAL SAFETY DATA SHEET

Section 6: ACCIDENTAL RELEASE MEASURES

Small Spill: Use appropriate tools to put the spilled solid in a convenient waste disposal container. Use respiratory protection and eye protection.

Large Spill: Use a shovel to put the material into a convenient waste disposal container. Vacuuming or wet sweeping may be used to avoid dust dispersal. Use respiratory protection and eye protection.

Section 7: HANDLING & STORAGE

Storage: Keep container tightly closed. Suitable for any general chemical storage area. Containers of this material may be hazardous when empty since they retain product residues (dust, solids); observe all warnings and precautions listed for the product.

Section 8: EXPOSURE CONTROLS / PERSONAL PROTECTION

Engineering Controls: Use process enclosures, local exhaust ventilation, or other engineering controls to keep airborne levels below recommended exposure limits. If user operations generate dust, fume or mist, use ventilation to keep exposure to airborne contaminants below the exposure limit. Personal Protection: Safety glasses. Lab coat. Respirator (NIOSH Approved). Gloves.

	Section 9: PHYSICAL & CHE	MICAL PROPERTIES		
Physical state:	Solid	Boling Point:	2230C (4046F)	
Color:	Yellow/Orange-Dry:Green-Saturated	Melting Point:	1610C (2930F)	
Odor:	Odorless	Vapor Pressure:	Not applicable.	
Solubility:	Insoluble	Vapor Density:	Not applicable.	
Specific Gravity:	2.1 (Water=1)	Evaporation Rate:	Not available.	
pH :	3 - 8 (in 5% slurry)		ime @ 21C (70F): 0	

Section 10: STABILITY & REACTIVITY

Stability: The product is stable.

Hazardous Decomposition Products: Oxides of carbon and silicon may be formed when heated. Hazardous Polymerization: Will not occur.

Incompatibility with powerfull oxiders: Reacts with hydrogen flouoride, fluorine, oxygen difluoride,

- chlorine trifluoride, strong acids, strong bases, and oxidizers.
- Conditions to Avoid: Moisture, extreme heat, and incompatibles.

Section 11: TOXICOLOGICAL INFORMATION

Routes of Entry: Absorbed through skin. Eye contact. Inhalation. Ingestion.

Toxicity to Animals:

LD50: Not available.

LC50: Not available.

Section 12: ECOLOGICAL INFORMATION

Ecotoxicity: This material is not expected to be toxic to aquatic life.

INTERRA Global Corporation

msds sSORB

p2

MATERIAL SAFETY DATA SHEET

Section 13: DISPOSAL CONSIDERATIONS Waste Disposal: Waste must be disposed of in accordance with federal, state and local environmental control regulations.

Section 14: TRANSPORT INFORMATION

DOT Classification: Not a DOT controlled material (United States). Identification: Not applicable.

Section 15: OTHER REGULATORY INFORMATION

HMIS (U.S.A.): Health Hazard: 1 Fire Hazard: 0 Reactivity: 0 Personal Protection: E National Fire Protection Association (U.S.A.): Health: 1 Flammability: 0 Reactivity: 0

Section 16: OTHER INFORMATION

References: Not available. Other Special Considerations: Not available.


 Created:
 04/03/2009
 11:20 AM

 Last Updated:
 03/25/2010
 10:40 AM

The purpose of this Safety Data Sheet is to describe the products in terms of their safety requirements. The information above is believed to be accurat and represents the bet information currently available to us. However, we make no warrant of merchantability or any other warranty, express or implied, with respect of such information, and we assume no liability resulting from its use. Users should make their own investigations to determine the suitability of the information for their particular purposes. In no event shal interra Global Corporation be liable for an claims, losses, or damages of any third party or for lost profits or any special, indirect, incidental, consequential or exemplary damages, howsoever arising, even if Interra Global Corporation has been advised of the possibility of such damages.

INTERRA Global Corporation

msds sSORB

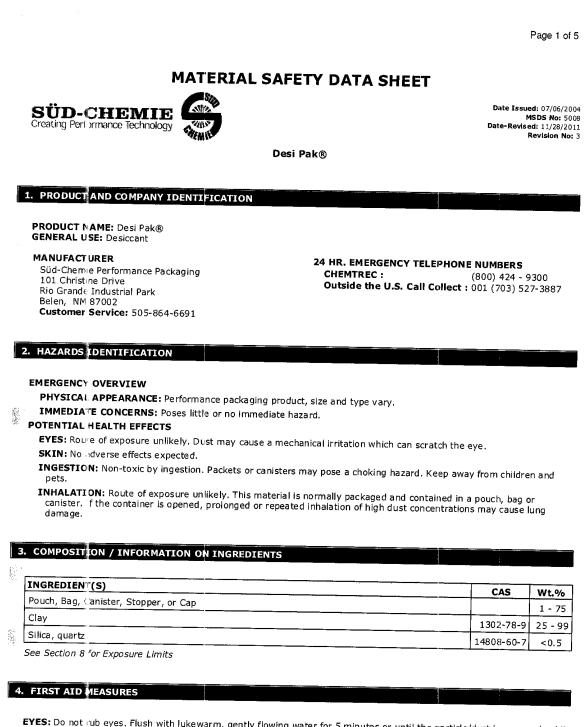

EYES: Do not nub eyes. Flush with lukewarm, gently flowing water for 5 minutes or until the particle/dust is removed, while holding the eyelid(s) open. Obtain medical attention. SKIN: Wash with soap and water.

23. 6

3

Page 2 of 5

Desi Pak®

- **INGESTION:** Normally not needed. If large quantities are ingested, call your local Poison Control Center (1-800-222-1222 in the U.S.)
- INHALATION: Normally not needed. If exposed to excessive levels of dust or fumes, remove to fresh air and seek medical attention of cough or other symptoms develop or persist.

5. FIRE FIGHTING MEASURES

FLASHPOINT AND METHOD: Material is not flammable

EXTINGUISHING MEDIA: Use extinguishing agent applicable to surrounding fire. **FIRE FIGHTING PROCEDURES:** As in any fire, wear celf-contained breathing apparatus operated in pressure-demand mode, (NIO3H approved or equivalent) and full protective gear.

6. ACCIDENTAL RELEASE MEASURES

SMALL SPILL: No special precautions required.

LARGE SPILL: With shovel or scoop, place material into appropriate container.

7. HANDLING AND STORAGE

HANDLING: Use of proper hygiene practices in the workplace is recommended.

STORAGE: Store in a dry area.

8. EXPOSURE CONTROLS / PERSONAL PROTECTION

EXPOSURE GUIDELINES HAZARDOUS COMPONENTS EXPOSURE LIMITS OSHA PEL ACGIH TLV mg/m³ mg/m³ ppm ppm Chemical Name [1] [1] [1] [1] TWA Clay 0.025 [3] [3] [2] [2] TWA Silica, quartz OSHA TABLE COMMENTS: 1. Exposure limits not established. **2.** Total Dust = (30 mg/m3)/(% SiO2+2)3. Respirable

ENGINEERING CONTROLS: If user operations generate dust, fume or mist, use ventilation to keep exposure to airborne contaminants below the exposure limit.

PERSONAL PROTECTIVE EQUIPMENT

ト

EYES AND FACE: Follow facility guidelines.

SKIN: Use of proper hygiene practices in the workplace is recommended.

RESPIRATORY: Use local exhaust if dusting occurs. Good general ventilation is adequate in the absence of dusts.

COMMENTS: All inert or nuisance dusts, whether mineral, inorganic, or organic, not listed specifically by substance name are covered by the Particulates Not Otherwise Regulated (PNOR) limit which is 5 mg/m3 for respirable fraction and 15 mg/m3 fo total dust. ACGIH exposure guidelines of less than 3 mg/m3 (respirable) and 10 mg/m3 (inhalable) have been established for particles (insoluble/poorly soluble) not otherwise specified (PNOS).

Desi Pak®

Page 3 of 5

9. PHYSICAL AND CHEMICAL PROPERTIES

PHYSICAL STATE: Solid ODOR: None pH: Not Determined PERCENT VOLATILE: None VAPOR PRESSURE: Not Applicable VAPOR DENSITY: Not applicable. EVAPORATION RATE: Not Applicable VISCOSITY: Not Applicable OXIDIZING PROPERTIES: None

10. STABILITY AND REACTIVITY

STABLE: Yes

HAZARDOUS POLYMERIZATION: No

11. TOXICOLOGICAL INFORMATION

Chemical Name	ORAL LD ₅₀	DERMAL LD ₅₀	INHALATION
	(rat)	(rabbit)	LC ₅₀ (rat)
Сіау	> 5000 gm/kg(b.w.)		> 200 mg/L/1H
Silica, qua tz	500	No Data	No Data
	gm/kg(b.w.)	Available	Available

CARCINOGENICITY

a.	Chemical Name	NTP Status	IARC Status	OSHA Status
	Clay	Not listed.	Not listed.	Not listed.
<i>.</i>	Silica, qua tz	Known Carcinogen	Group I	Not listed.

SENSITIZAT (ON: Not sensitizing

GENERAL COMMENTS: Crystalline silica present is contained within a pouch, canister or bag. No exposure to airborne particles of respirable size is expected under normal conditions of use.

12. ECOLOGICAL INFORMATION

ENVIRONMENTAL DATA: Low hazard for usual industrial or commercial handling. CHEMICAL FATE INFORMATION: This material is of mineral origin. It is not biodegradable.

13. DISPOSAL CONSIDERATIONS

DISPOSAL METHOD: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Processing, use or

記録

	contamination of this product may change the waste management options. State and local di from federal disposal regulations.	isposal re	gulations may d
1	14. TRANSPORT INFORMATION		
	DOT (DEPARTMENT OF TRANSPORTATION)		·····
	PROPER SHIPPING NAME: Not regulated		
	ROAD AND RAIL (ADR/RID)		
	PROPER SHIPPING NAME: Not regulated		
	AIR (ICAO/IATA)		
	SHIPPING NAME: Not regulated		
	VESSEL (IMO/IMDG)		
	SHIPPING NAME: Not regulated		
	CANADA TRANSPORT OF DANGEROUS GOODS		
	SHIPPING NAME: Not regulated		
	5. REGULATORY INFORMATION		
(UNITED STATES		
	SARA TITLE III (SUPERFUND AMENDMENTS AND REAUTHORIZATION ACT)		
	FIRE: NO PRESSURE GENERATING: NO REACTIVITY: NO ACUTE: NO CHRONICS Y	(a.e.	
	313 050 0074 DI - 20000	es	
	SIS REFORTABLE INGREDIENTS: Not listed.		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT)		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed.		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT)		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TO)CIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS		
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TO)CIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain should be a set of the state of the second set of the second s	:.	ifornia to cause
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California	:. ate of Cal	
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, birth defects, or reproductive harm. Crystalline silica present is contained within a pouch consistence begin T	t. ate of Cali	particles of
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the stat cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use,	t. ate of Cal airborne	particles of
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc	t. ate of Cal. airborne Wt.% <0.5	particles of Listed Cancer
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations.	t. ate of Cal. airborne Wt.% <0.5	particles of Listed Cancer
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations.	t. ate of Cal. airborne Wt.% <0.5	particles of Listed Cancer
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations.	t. ate of Cal. airborne Wt.% <0.5	particles of Listed Cancer
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, birth defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations. ANADA WHMIS HA?ARD SYMBOL AND CLASSIFICATION	ate of Cal airborne Wt.% <0.5 cessing, u sposal reg	Listed Cancer Use or gulations may
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, birth defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations. ANADA WHMIS HAZARD SYMBOL AND CLASSIFICATION Doe: not meet classification criteria pursuant to the Canadian Hazardous Products Act. WHMIS (WORKPLACE HAZARDOUS MATERIALS INFORMATION SYSTEM): This MSDS has according to the hazard criteria of the Controlled Products Regulations (CPR) and the MSDS co information required by the CPR.	ate of Cal airborne Wt.% <0.5 cessing, u sposal reg	eparticles of Listed Cancer use or gulations may
	CERCLA (COMPREHENSIVE RESPONSE, COMPENSATION, AND LIABILITY ACT) CERCLA REGULATORY: Not listed. TSCA (TOXIC SUBSTANCE CONTROL ACT) TSCA STATUS: All components are listed on the TSCA Inventory or are excluded or exempt REGULATIONS STATE REGULATIONS: California CALIFORNIA PROPOSITION 65: This product does not contain chemical(s) known to the sta cancer, bit th defects, or reproductive harm. Crystalline silica present is contained within a pouch, canister or bag. There is no exposure to respirable size under normal conditions of use. Chemical Name Silica, quartz RCRA STATUS: This product, if discarded as sold, is not a Federal RCRA hazardous waste. Proc contamination of this product may change the waste management options. State and local dis differ from federal disposal regulations. ANADA WHMIS HAZARD SYMBOL AND CLASSIFICATION Doe: not meet classification criteria pursuant to the Canadian Hazardous Products Act. WHMIS (WORKPLACE HAZARDOUS MATERIALS INFORMATION SYSTEM): This MSDS has according to the hazard criteria of the Controlled Derothyle Control of the provention of the controlled Derothyle Control of the hazard criteria of the Controlled Derothyle Control of the provention of the controlled Derothyle Control of the provention of the controlled Derothyle Control of the provention of the controlled Derothyle Control of the controlled Derothyle Control of the controlled Derothyle Control of the provention of the controlled Derothyle Control of the controlled Derothyle Control of the controlled Derothyle Control of the provention of the controlled Derothyle Control of the controlled Derothyle Controlled Derothyle Control o	ate of Cal airborne Wt.% <0.5 cessing, u sposal reg s been pr intains all ozardous l	eparticles of Listed Cancer use or gulations may epared of the Products Act

Page 5 of 5

EUROPEAN COMMUNITY EEC LABEL SYMBOL AND CLASSIFICATION

Not classified as dangerous


16. OTHER INFORMATION


Desi Pak®

N)

APPROVED BY: Prepared and approved by SHE Dept. Sud-Chemie Inc.

- INFORMATION CONTACT: E-mail MSDS_US@sud-chemie.com
- REVISION SUMMARY: This MSDS replaces the 01/21/2009 MSDS. Revised: Section 1: INFORMATION CONTACT. Section 16: HMIS RATING (HEALTH, PHYSICAL HAZARD, HMIS RATINGS NOTES, CHRONIC).





HMIS RATINGS NOTES: Personal Protection should be determined based on workplace conditions.

MANUFACTURER DISCLAIMER: The information presented herein is believed to be accurate but is not warranted. Recipients are advised to confirm in advance that the information is current, applicable and suitable to their circumstances.